

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
 Data File : BG051470.D
 Acq On : 11 Dec 2021 1:08
 Operator : CG/JU
 Sample : M4985-19
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW5R0

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/13/2021
 Supervised By :Yogesh Patel 12/15/2021

Quant Time: Dec 11 04:26:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 09 03:21:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.185	152	24011	20.000	ng/u1	0.00
20) Naphthalene-d8	11.011	136	108174	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.818	164	73282	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.568	188	161314	20.000	ng/u1	0.00
79) Chrysene-d12	21.875	240	140121	20.000	ng/u1	0.00
88) Perylene-d12	25.265	264	131627	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.531	96	4086	5.588	ng/uL	0.00
4) Pyridine-d5	4.007	84	8209m	3.910	ng/u1	0.04
7) Phenol-d5	7.392	99	10181	4.165	ng/u1	0.04
9) Bis-(2-Chloroethyl)eth...	7.503	67	49779	31.756	ng/u1	0.00
11) 2-Chlorophenol-d4	7.732	132	38092	21.904	ng/u1	0.00
15) 4-Methylphenol-d8	8.931	113	22322	11.624	ng/u1	0.02
21) Nitrobenzene-d5	9.372	128	29587	31.530	ng/u1	0.00
24) 2-Nitrophenol-d4	10.100	143	30658	28.872	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.658	165	38805	22.464	ng/u1	0.00
31) 4-Chloroaniline-d4	11.170	131	58428	23.125	ng/u1	0.00
46) Dimethylphthalate-d6	14.213	166	207793	36.645	ng/u1	0.00
49) Acenaphthylene-d8	14.513	160	254135	35.387	ng/u1	0.00
54) 4-Nitrophenol-d4	15.200	143	1972m	2.310	ng/u1	0.14
60) Fluorene-d10	15.805	176	189720	37.585	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.958	200	27881	29.085	ng/u1	0.00
73) Anthracene-d10	17.668	188	316614	41.948	ng/u1	0.00
81) Pyrene-d10	19.948	212	355685	42.232	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.030	264	305080	44.936	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.698	149	41197	6.683	ng/u1	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
Data File : BG051470.D
Acq On : 11 Dec 2021 1:08
Operator : CG/JU
Sample : M4985-19
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
EW5R0

Quant Time: Dec 11 04:26:37 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 09 03:21:41 2021
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/13/2021
Supervised By :Yogesh Patel 12/15/2021

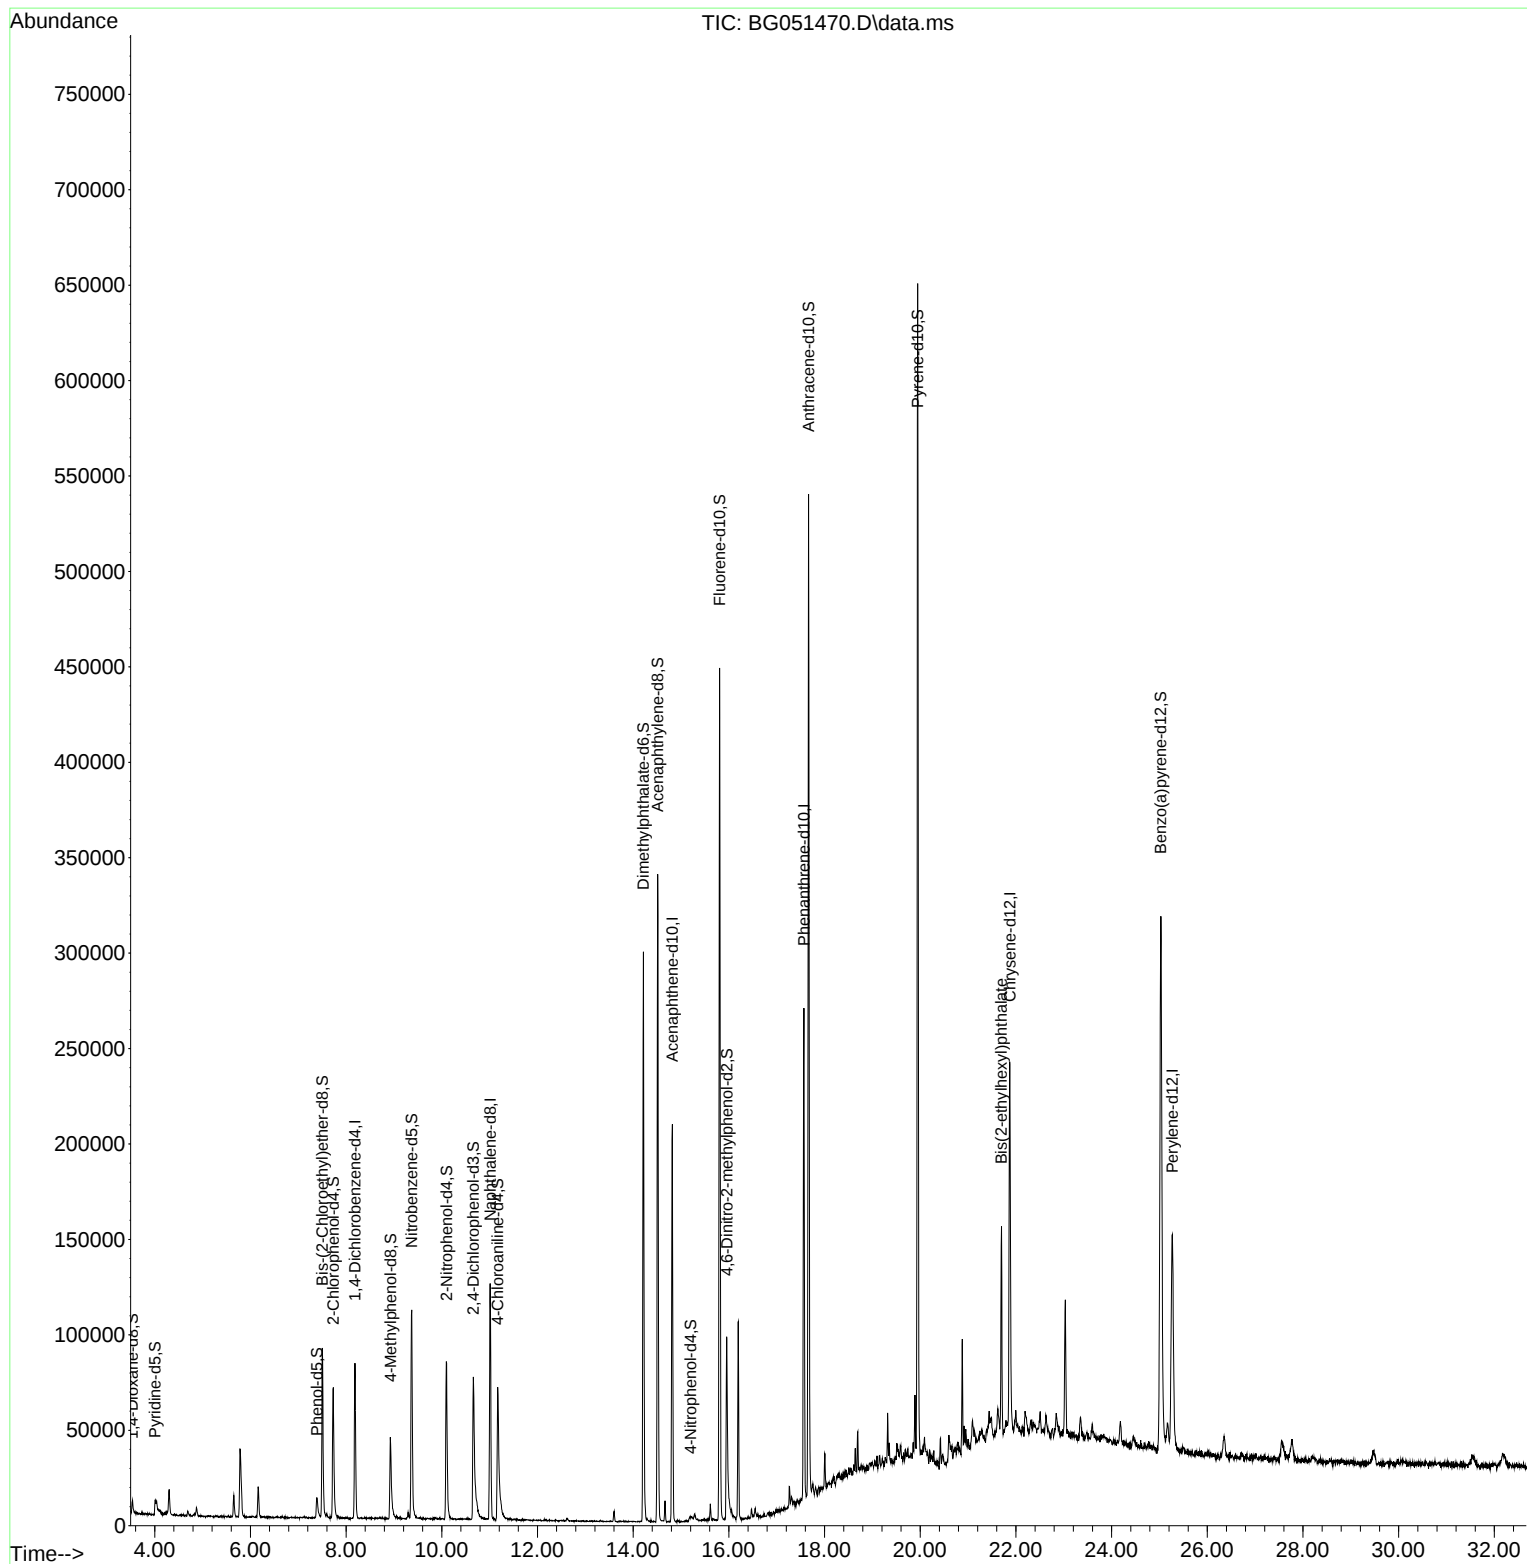

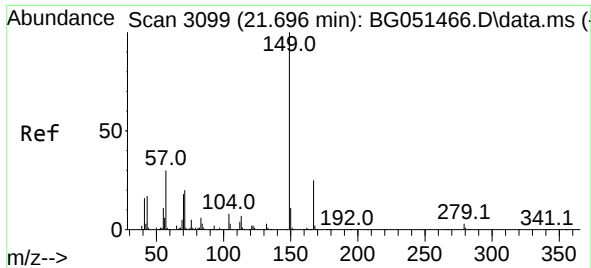

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 6.683 ng/ul
 RT: 21.698 min Scan# 3099
 Delta R.T. -0.010 min
 Lab File: BG051470.D
 Acq: 11 Dec 2021 1:08

Instrument :
 BNA_G
 ClientSampleId :
 EW5R0

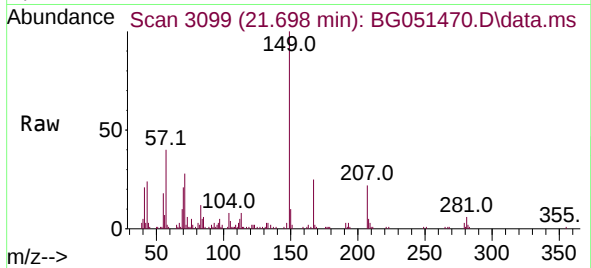

Tgt Ion:149 Resp: 4119
 Ion Ratio Lower Upper
 149 100
 167 25.4 21.1 31.7
 279 3.5 2.7 4.1

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/13/2021
 Supervised By :Yogesh Patel 12/15/2021

