

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
 Data File : BG051471.D
 Acq On : 11 Dec 2021 1:49
 Operator : CG/JU
 Sample : M4985-20
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW5R6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/13/2021
 Supervised By :Yogesh Patel 12/15/2021

Quant Time: Dec 11 04:27:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 09 03:21:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.185	152	23059	20.000	ng/u1	0.00
20) Naphthalene-d8	11.011	136	100165	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.818	164	68632	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.568	188	149814	20.000	ng/u1	0.00
79) Chrysene-d12	21.875	240	132607	20.000	ng/u1	0.00
88) Perylene-d12	25.265	264	128247	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.531	96	3615	5.148	ng/uL	0.00
4) Pyridine-d5	3.995	84	13556m	6.723	ng/u1	0.03
7) Phenol-d5	7.380	99	13542	5.769	ng/u1	0.03
9) Bis-(2-Chloroethyl)eth...	7.503	67	52542	34.903	ng/u1	0.00
11) 2-Chlorophenol-d4	7.726	132	42821	25.639	ng/u1	0.00
15) 4-Methylphenol-d8	8.925	113	28660	15.541	ng/u1	0.01
21) Nitrobenzene-d5	9.366	128	31051	35.736	ng/u1	0.00
24) 2-Nitrophenol-d4	10.094	143	32971	33.533	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.658	165	47523	29.710	ng/u1	0.00
31) 4-Chloroaniline-d4	11.169	131	57142	24.424	ng/u1	0.00
46) Dimethylphthalate-d6	14.213	166	203623	38.342	ng/u1	0.00
49) Acenaphthylene-d8	14.513	160	253589	37.703	ng/u1	0.00
54) 4-Nitrophenol-d4	15.194	143	2532m	3.167	ng/u1	0.13
60) Fluorene-d10	15.805	176	186626	39.477	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.952	200	30905	34.715	ng/u1	0.00
73) Anthracene-d10	17.668	188	308191	43.966	ng/u1	0.00
81) Pyrene-d10	19.947	212	356395	44.714	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.030	264	305860	46.239	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.698	149	44604	7.645	ng/u1	Qvalue 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
Data File : BG051471.D
Acq On : 11 Dec 2021 1:49
Operator : CG/JU
Sample : M4985-20
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
EW5R6

Quant Time: Dec 11 04:27:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 09 03:21:41 2021
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/13/2021
Supervised By :Yogesh Patel 12/15/2021

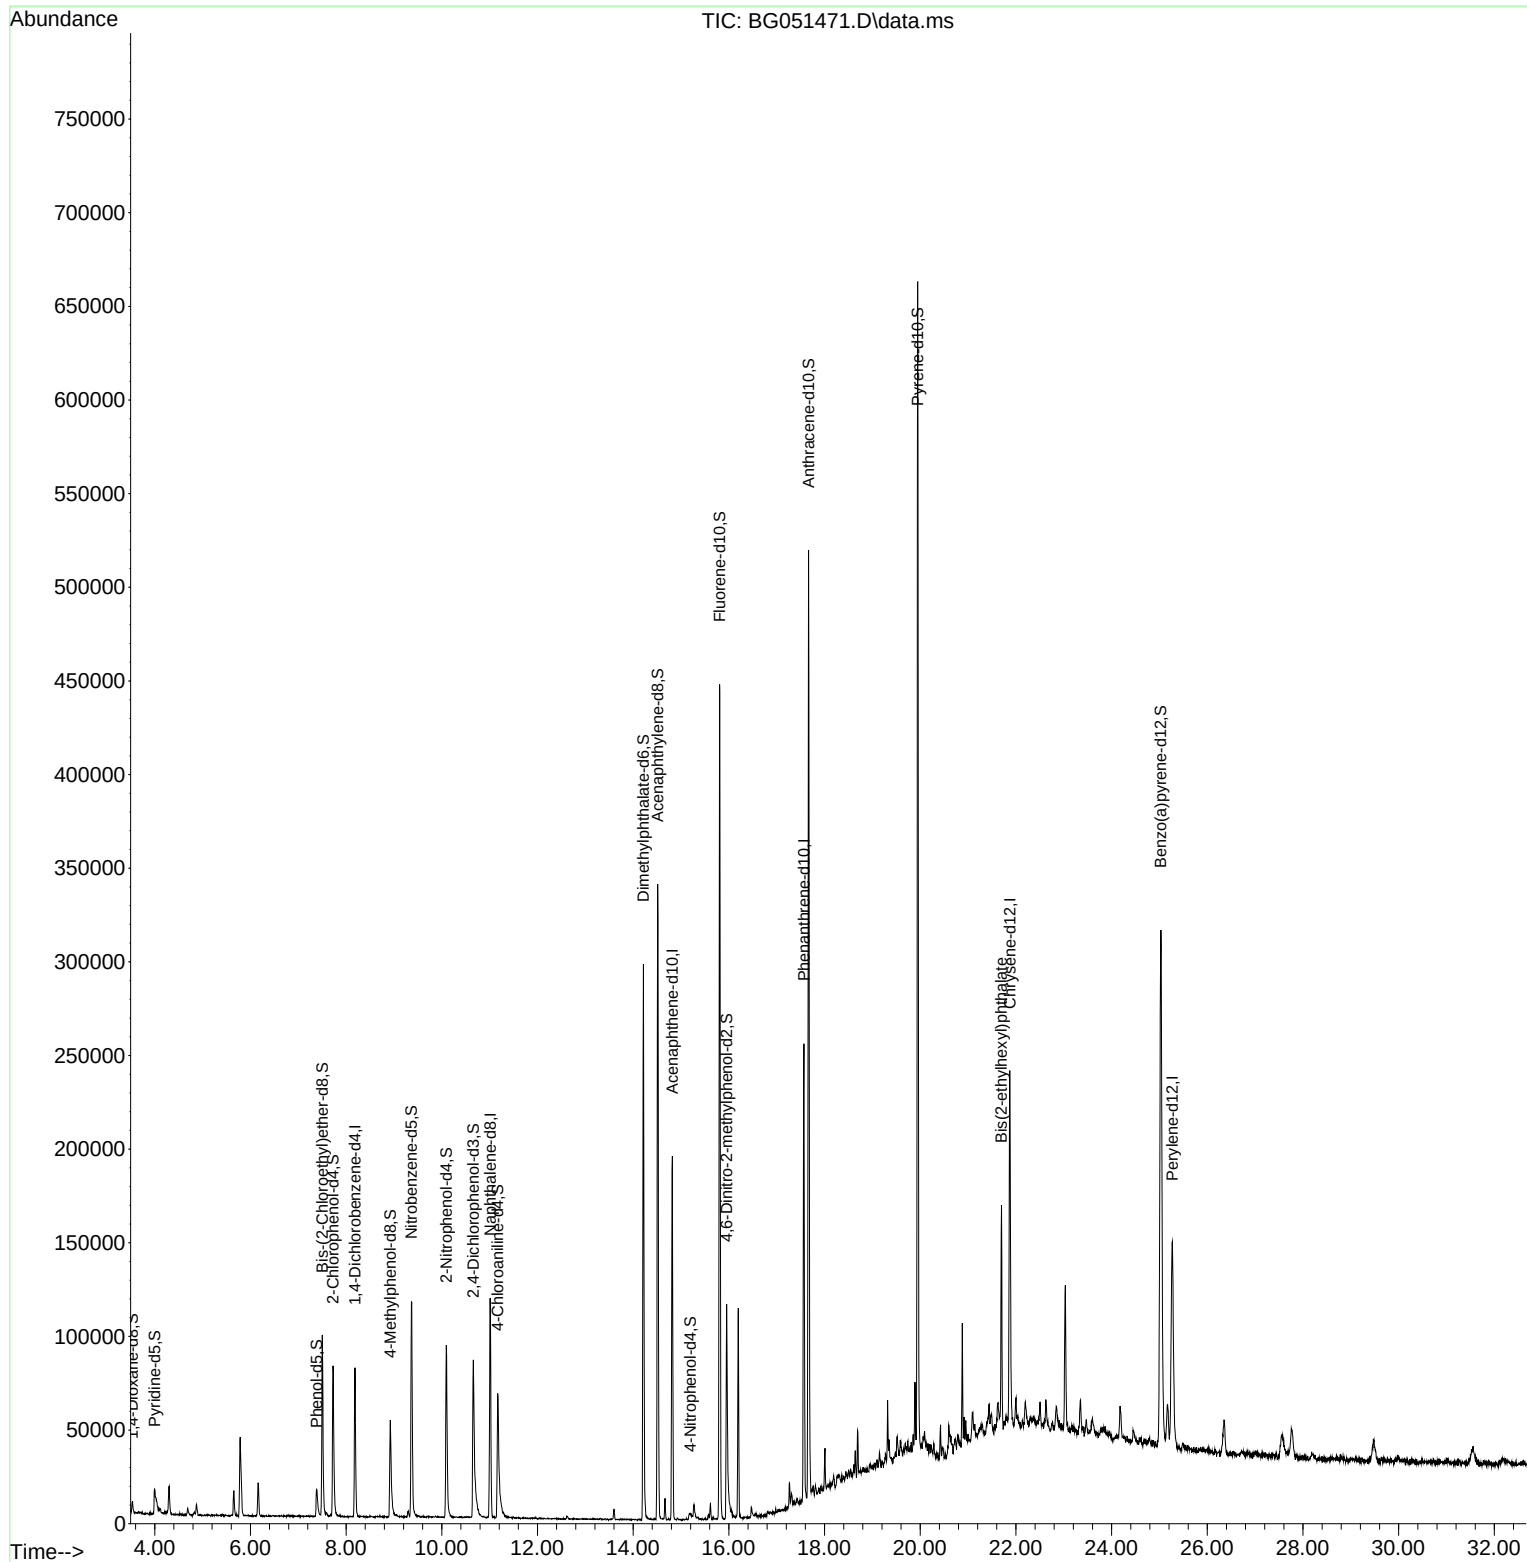

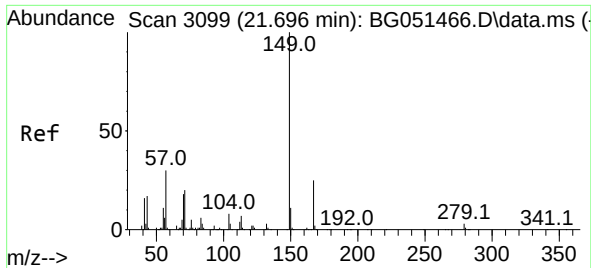

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 7.645 ng/ul
 RT: 21.698 min Scan# 3099
 Delta R.T. -0.010 min
 Lab File: BG051471.D
 Acq: 11 Dec 2021 1:49

Instrument :
 BNA_G
 ClientSampleId :
 EW5R6

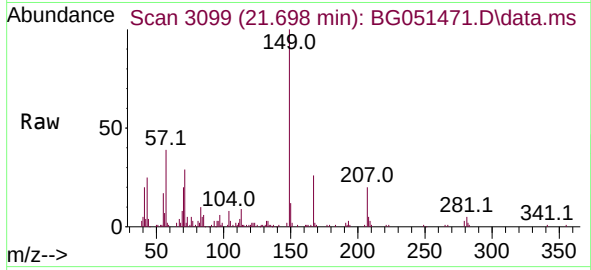

Tgt Ion:	149	Resp:	44604
Ion Ratio	Lower	Upper	
149	100		
167	26.3	21.1	31.7
279	3.3	2.7	4.1

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/13/2021
 Supervised By :Yogesh Patel 12/15/2021

