

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
 Data File : BG051472.D
 Acq On : 11 Dec 2021 2:30
 Operator : CG/JU
 Sample : M4985-21
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW5S6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/13/2021
 Supervised By :Yogesh Patel 12/15/2021

Quant Time: Dec 11 04:28:02 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 09 03:21:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.188	152	23333	20.000	ng/u1	0.00
20) Naphthalene-d8	11.008	136	104288	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.816	164	70327	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.565	188	160200	20.000	ng/u1	0.00
79) Chrysene-d12	21.872	240	147617	20.000	ng/u1	0.00
88) Perylene-d12	25.268	264	141274	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.535	96	3461	4.871	ng/uL	0.00
4) Pyridine-d5	3.999	84	8911m	4.367	ng/u1	0.03
7) Phenol-d5	7.389	99	12758	5.371	ng/u1	0.03
9) Bis-(2-Chloroethyl)eth...	7.501	67	49010	32.174	ng/u1	0.00
11) 2-Chlorophenol-d4	7.730	132	40543	23.990	ng/u1	0.00
15) 4-Methylphenol-d8	8.923	113	26853	14.390	ng/u1	0.01
21) Nitrobenzene-d5	9.369	128	28781	31.814	ng/u1	0.00
24) 2-Nitrophenol-d4	10.098	143	30467	29.762	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.662	165	44195	26.538	ng/u1	0.01
31) 4-Chloroaniline-d4	11.173	131	53664	22.031	ng/u1	0.01
46) Dimethylphthalate-d6	14.216	166	188522	34.643	ng/u1	0.00
49) Acenaphthylene-d8	14.516	160	240165	34.846	ng/u1	0.00
54) 4-Nitrophenol-d4	15.215	143	1620m	1.977	ng/u1	0.15
60) Fluorene-d10	15.809	176	174520	36.026	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.961	200	16671	17.512	ng/u1	0.01
73) Anthracene-d10	17.665	188	299716	39.985	ng/u1	0.00
81) Pyrene-d10	19.945	212	349213	39.358	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.027	264	304082	41.731	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.696	149	47135	7.258	ng/u1	Qvalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
Data File : BG051472.D
Acq On : 11 Dec 2021 2:30
Operator : CG/JU
Sample : M4985-21
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
EW5S6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/13/2021
Supervised By :Yogesh Patel 12/15/2021


Quant Time: Dec 11 04:28:02 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 09 03:21:41 2021
Response via : Initial Calibration

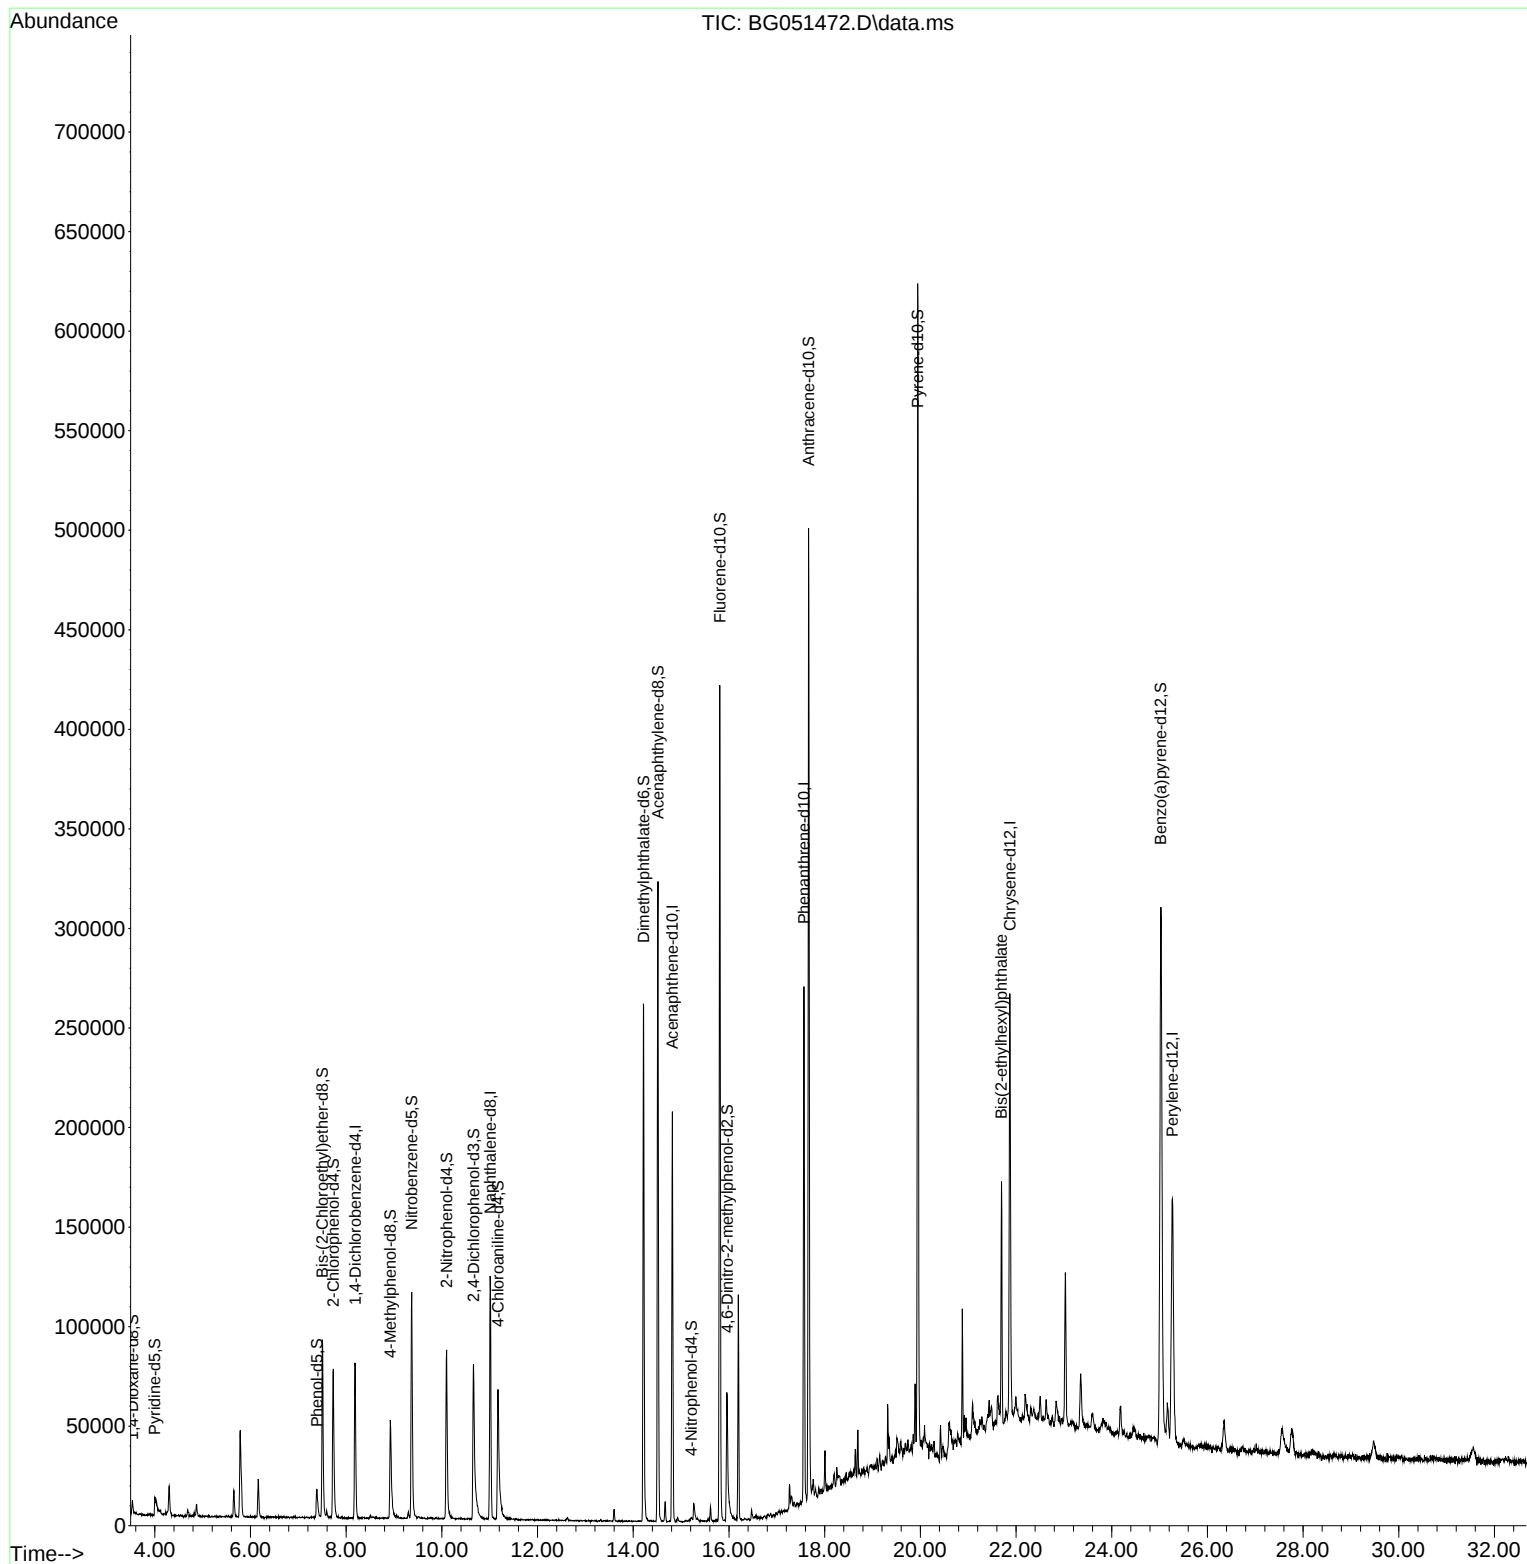

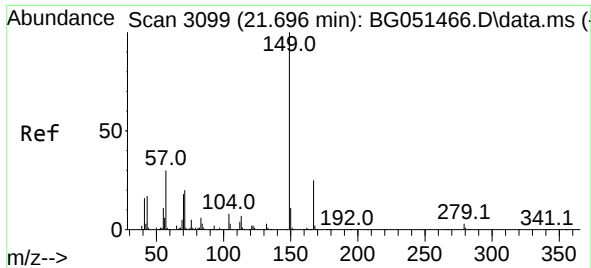

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 7.258 ng/ul
 RT: 21.696 min Scan# 3099
 Delta R.T. -0.012 min
 Lab File: BG051472.D
 Acq: 11 Dec 2021 2:30

Instrument :
 BNA_G
 ClientSampleId :
 EW5S6

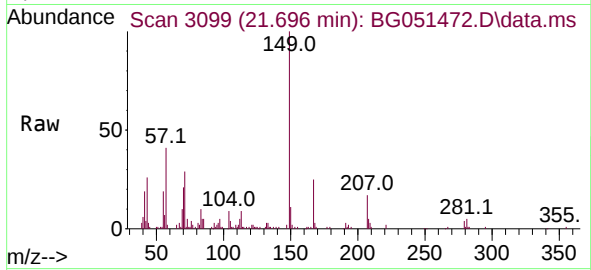

Tgt Ion:149 Resp: 47135
 Ion Ratio Lower Upper
 149 100
 167 24.8 21.1 31.7
 279 3.5 2.7 4.1

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/13/2021
 Supervised By :Yogesh Patel 12/15/2021

