

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
 Data File : BG051428.D
 Acq On : 9 Dec 2021 10:37
 Operator : CG/JU
 Sample : PB141216BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK216

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051428.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.529	3	7	15	rVB2	7470	11736	1.47%	0.149%
2	3.888	65	68	70	rVB2	1042	939	0.12%	0.012%
3	3.970	77	82	99	rBV	75722	163146	20.44%	2.069%
4	4.176	116	117	120	rVB3	1073	926	0.12%	0.012%
5	4.299	135	138	144	rVB6	1590	3068	0.38%	0.039%
6	4.464	163	166	169	rBV2	866	1114	0.14%	0.014%
7	4.558	179	182	184	rBV3	761	906	0.11%	0.011%
8	5.086	270	272	275	rVB2	941	977	0.12%	0.012%
9	5.280	303	305	309	rBV3	680	1071	0.13%	0.014%
10	6.179	456	458	460	rVB2	837	823	0.10%	0.010%
11	6.355	485	488	492	rBV	775	1145	0.14%	0.015%
12	6.955	586	590	591	rBV2	750	1115	0.14%	0.014%
13	7.360	653	659	677	rBV	98663	204701	25.65%	2.596%
14	7.507	677	684	693	rVB	86845	153874	19.28%	1.951%
15	7.724	714	721	734	rBV	106798	199262	24.96%	2.527%
16	8.189	793	800	809	rVB	91036	155873	19.53%	1.977%
17	8.911	917	923	940	rVV	125882	245226	30.72%	3.110%
18	9.370	994	1001	1011	rBV	112036	208484	26.12%	2.644%
19	10.098	1118	1125	1137	rBV	92412	178582	22.37%	2.265%
20	10.656	1213	1220	1243	rBV	96476	231444	29.00%	2.935%
21	11.015	1274	1281	1293	rVB	130850	238725	29.91%	3.027%
22	11.162	1300	1306	1326	rBV	105849	250741	31.41%	3.180%
23	12.619	1549	1554	1557	rBV2	1912	3106	0.39%	0.039%
24	13.194	1649	1652	1657	rVB2	579	957	0.12%	0.012%
25	13.676	1731	1734	1737	rVV2	625	838	0.10%	0.011%
26	13.712	1737	1740	1743	rVB2	594	892	0.11%	0.011%
27	14.158	1811	1816	1818	rBV2	616	863	0.11%	0.011%
28	14.217	1820	1826	1839	rVV	271415	417213	52.27%	5.291%
29	14.522	1871	1878	1889	rVV	301133	491976	61.64%	6.239%
30	14.616	1891	1894	1899	rVB3	620	1018	0.13%	0.013%
31	14.822	1922	1929	1940	rVB	216599	344582	43.17%	4.370%
32	15.086	1969	1974	1989	rBV3	38588	121411	15.21%	1.540%
33	15.815	2091	2098	2108	rBV	383193	611584	76.62%	7.756%
34	15.956	2117	2122	2138	rBV	69456	141041	17.67%	1.789%
35	16.056	2138	2139	2145	rVB2	2958	3348	0.42%	0.042%
36	16.655	2238	2241	2243	rVB	936	862	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
 Data File : BG051428.D
 Acq On : 9 Dec 2021 10:37
 Operator : CG/JU
 Sample : PB141216BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK216

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
 Title : SVOA CALIBRATION

37	16.920	2281	2286	2289	rVB2	807	1016	0.13%	0.013%
38	17.372	2356	2363	2367	rBV4	908	1640	0.21%	0.021%
39	17.472	2376	2380	2383	rVB2	691	948	0.12%	0.012%
40	17.572	2391	2397	2406	rBV	295270	436718	54.71%	5.538%
41	17.672	2408	2414	2427	rVB2	429230	688626	86.27%	8.733%
42	18.347	2526	2529	2532	rBV3	734	975	0.12%	0.012%
43	18.794	2602	2605	2608	rBV3	606	849	0.11%	0.011%
44	18.905	2621	2624	2625	rBV2	1177	1160	0.15%	0.015%
45	18.982	2636	2637	2641	rVB3	1284	1177	0.15%	0.015%
46	19.029	2643	2645	2648	rBV3	789	922	0.12%	0.012%
47	19.082	2650	2654	2655	rBV3	1008	1073	0.13%	0.014%
48	19.246	2679	2682	2685	rBV	680	973	0.12%	0.012%
49	19.311	2691	2693	2696	rBV4	947	1335	0.17%	0.017%
50	19.340	2696	2698	2701	rVV3	916	1045	0.13%	0.013%
51	19.375	2702	2704	2707	rVV2	945	992	0.12%	0.013%
52	19.522	2725	2729	2732	rBV4	6029	8815	1.10%	0.112%
53	19.593	2737	2741	2746	rVB2	5364	7739	0.97%	0.098%
54	19.687	2755	2757	2759	rBV3	878	827	0.10%	0.010%
55	19.834	2780	2782	2784	rBV3	1374	1432	0.18%	0.018%
56	19.951	2796	2802	2814	rBV2	511770	798202	100.00%	10.123%
57	20.075	2822	2823	2825	rBV2	1390	1334	0.17%	0.017%
58	20.175	2837	2840	2841	rBV3	1804	1725	0.22%	0.022%
59	20.274	2855	2857	2858	rBV2	2129	1554	0.19%	0.020%
60	20.333	2865	2867	2869	rBV3	1588	1705	0.21%	0.022%
61	20.398	2876	2878	2879	rBV	2060	1669	0.21%	0.021%
62	20.574	2906	2908	2909	rBV	1897	1449	0.18%	0.018%
63	20.715	2928	2932	2933	rBV4	4778	5135	0.64%	0.065%
64	20.856	2953	2956	2957	rBV3	2615	3048	0.38%	0.039%
65	21.873	3123	3129	3142	rVB2	223840	435945	54.62%	5.529%
66	25.039	3657	3668	3681	rBV2	227791	683545	85.64%	8.669%
67	25.280	3699	3709	3720	rVB	127123	395011	49.49%	5.009%
68	27.454	4077	4079	4081	rBV2	4006	3194	0.40%	0.041%




Sum of corrected areas: 7885347

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
Data File : BG051428.D
Acq On : 9 Dec 2021 10:37
Operator : CG/JU
Sample : PB141216BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK216

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

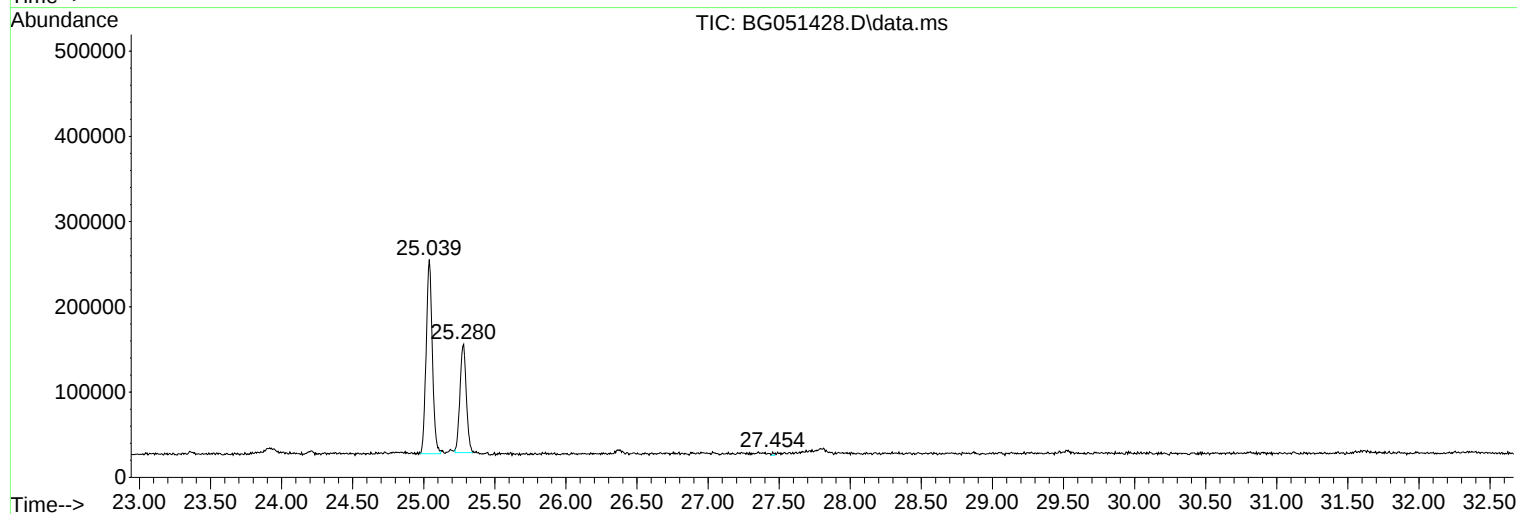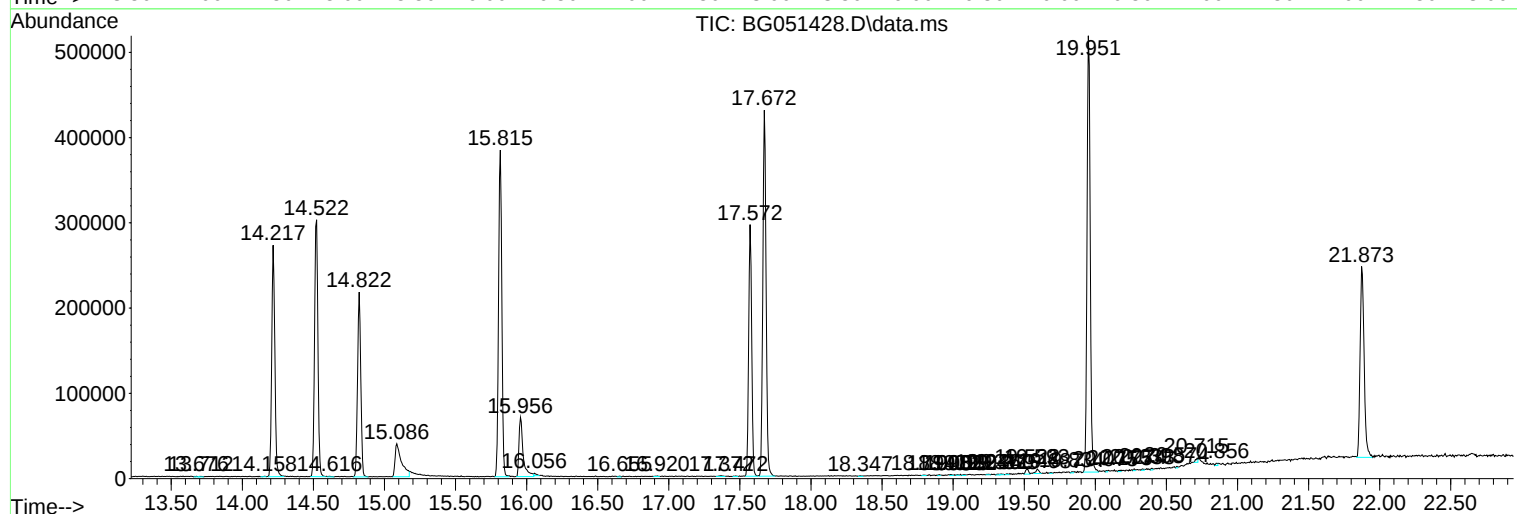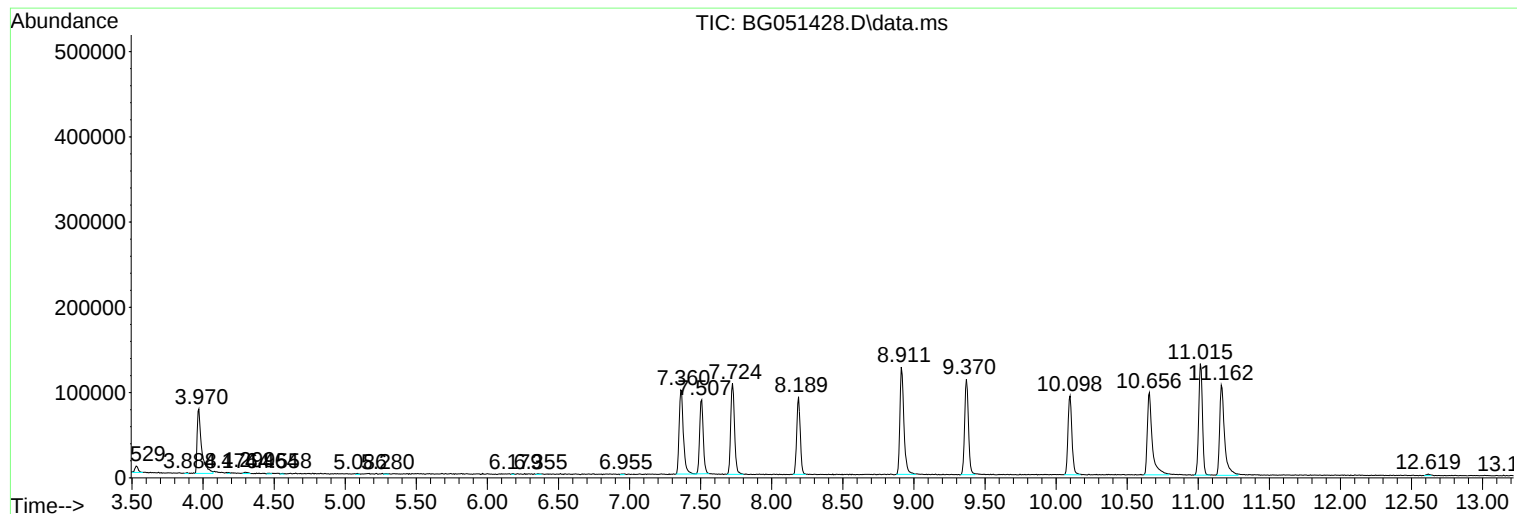

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
Data File : BG051428.D
Acq On : 9 Dec 2021 10:37
Operator : CG/JU
Sample : PB141216BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK216

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
Data File : BG051428.D
Acq On : 9 Dec 2021 10:37
Operator : CG/JU
Sample : PB141216BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK216

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
