

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
 Data File : BG051441.D
 Acq On : 9 Dec 2021 21:29
 Operator : CG/JU
 Sample : PB141217BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK217

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051441.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.530	3	7	16	rVB2	7374	12541	1.54%	0.159%
2	3.971	78	82	100	rBV	73357	158511	19.49%	2.014%
3	4.300	134	138	142	rBV3	1161	1991	0.24%	0.025%
4	5.540	347	349	351	rBV	936	965	0.12%	0.012%
5	6.592	524	528	531	rBV2	967	1741	0.21%	0.022%
6	6.686	541	544	547	rVB3	644	876	0.11%	0.011%
7	7.150	619	623	624	rBV3	930	1220	0.15%	0.015%
8	7.361	653	659	671	rBV	102576	207802	25.55%	2.640%
9	7.502	677	683	695	rVB	90141	157468	19.36%	2.000%
10	7.720	714	720	731	rBV	104920	201403	24.76%	2.558%
11	8.184	792	799	808	rBV	83658	146538	18.02%	1.862%
12	8.912	917	923	939	rBV2	124970	257979	31.72%	3.277%
13	9.106	954	956	961	rVB3	853	1049	0.13%	0.013%
14	9.288	984	987	990	rVB2	706	878	0.11%	0.011%
15	9.365	993	1000	1011	rVV	110879	213783	26.28%	2.716%
16	9.435	1011	1012	1016	rVV2	1730	2208	0.27%	0.028%
17	9.523	1025	1027	1031	rBV2	799	826	0.10%	0.010%
18	9.612	1039	1042	1045	rBV2	600	923	0.11%	0.012%
19	10.093	1117	1124	1135	rBV	93232	181395	22.30%	2.304%
20	10.651	1213	1219	1244	rBV	97756	237089	29.15%	3.012%
21	11.010	1273	1280	1288	rBV	121581	223499	27.48%	2.839%
22	11.163	1299	1306	1323	rBV	105111	251560	30.93%	3.196%
23	12.620	1548	1554	1562	rBV4	1889	3989	0.49%	0.051%
24	13.536	1707	1710	1715	rBV2	568	991	0.12%	0.013%
25	14.212	1819	1825	1836	rBV	262008	419922	51.63%	5.334%
26	14.518	1870	1877	1887	rBV	297017	493308	60.65%	6.267%
27	14.817	1922	1928	1939	rVB	204808	326972	40.20%	4.154%
28	15.087	1969	1974	1992	rBV4	38181	132532	16.29%	1.684%
29	15.387	2022	2025	2030	rVB5	769	1202	0.15%	0.015%
30	15.810	2090	2097	2106	rBV	384604	614150	75.50%	7.802%
31	15.951	2116	2121	2135	rBV	81214	159033	19.55%	2.020%
32	16.045	2135	2137	2140	rVB4	1787	2432	0.30%	0.031%
33	16.603	2228	2232	2235	rBV2	496	850	0.10%	0.011%
34	17.355	2357	2360	2362	rBV3	833	1134	0.14%	0.014%
35	17.567	2390	2396	2403	rVV	267735	408822	50.26%	5.193%
36	17.667	2407	2413	2426	rVB2	410262	683452	84.02%	8.682%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
 Data File : BG051441.D
 Acq On : 9 Dec 2021 21:29
 Operator : CG/JU
 Sample : PB141217BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK217

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
 Title : SVOA CALIBRATION

37	18.525	2557	2559	2563	rVV2	826	833	0.10%	0.011%
38	19.476	2719	2721	2723	rBV3	1312	1432	0.18%	0.018%
39	19.518	2723	2728	2731	rVV4	6036	8850	1.09%	0.112%
40	19.594	2734	2741	2745	rVV3	5138	9146	1.12%	0.116%
41	19.747	2766	2767	2769	rVB	1793	846	0.10%	0.011%
42	19.770	2769	2771	2772	rBV2	1343	1103	0.14%	0.014%
43	19.835	2781	2782	2784	rVB2	1222	847	0.10%	0.011%
44	19.946	2795	2801	2815	rBV	514361	813392	100.00%	10.333%
45	20.111	2828	2829	2830	rBV	1796	819	0.10%	0.010%
46	20.299	2858	2861	2862	rBV2	1867	1649	0.20%	0.021%
47	20.411	2879	2880	2883	rBV3	1856	2247	0.28%	0.029%
48	20.669	2913	2924	2930	rBV3	7955	35709	4.39%	0.454%
49	21.380	3043	3045	3046	rBV2	3916	2995	0.37%	0.038%
50	21.874	3122	3129	3141	rVB	210712	411362	50.57%	5.226%
51	25.029	3656	3666	3680	rBV2	227916	685709	84.30%	8.711%
52	25.270	3697	3707	3724	rVB4	118233	384014	47.21%	4.878%



Sum of corrected areas: 7871987

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
Data File : BG051441.D
Acq On : 9 Dec 2021 21:29
Operator : CG/JU
Sample : PB141217BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK217

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

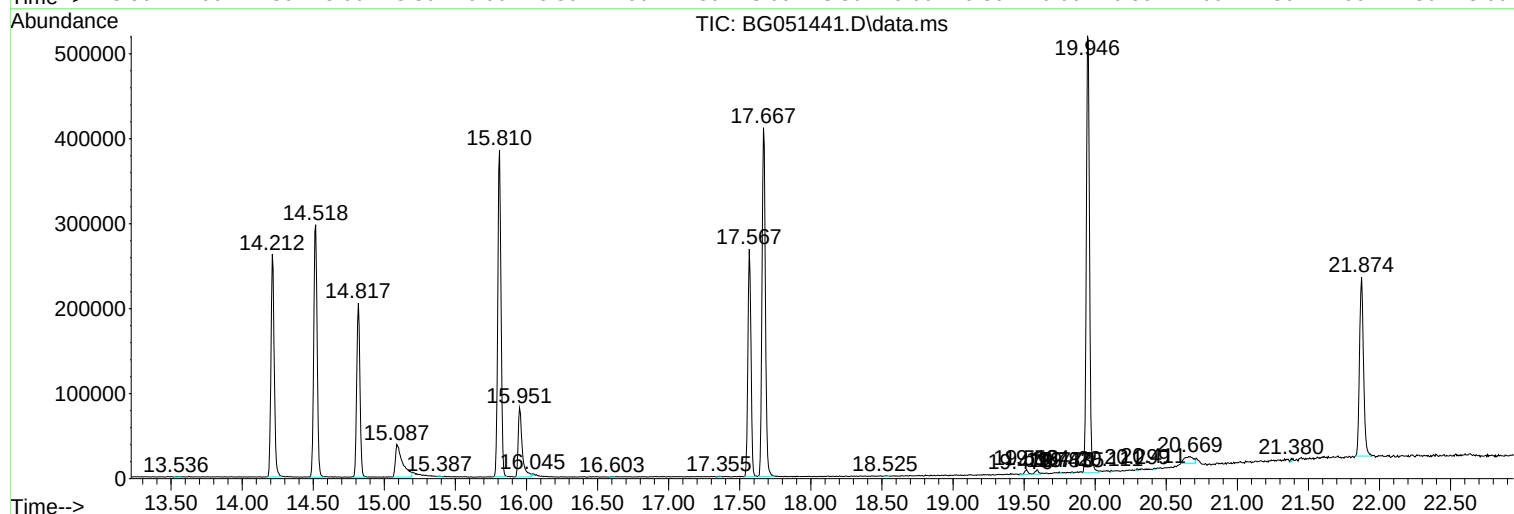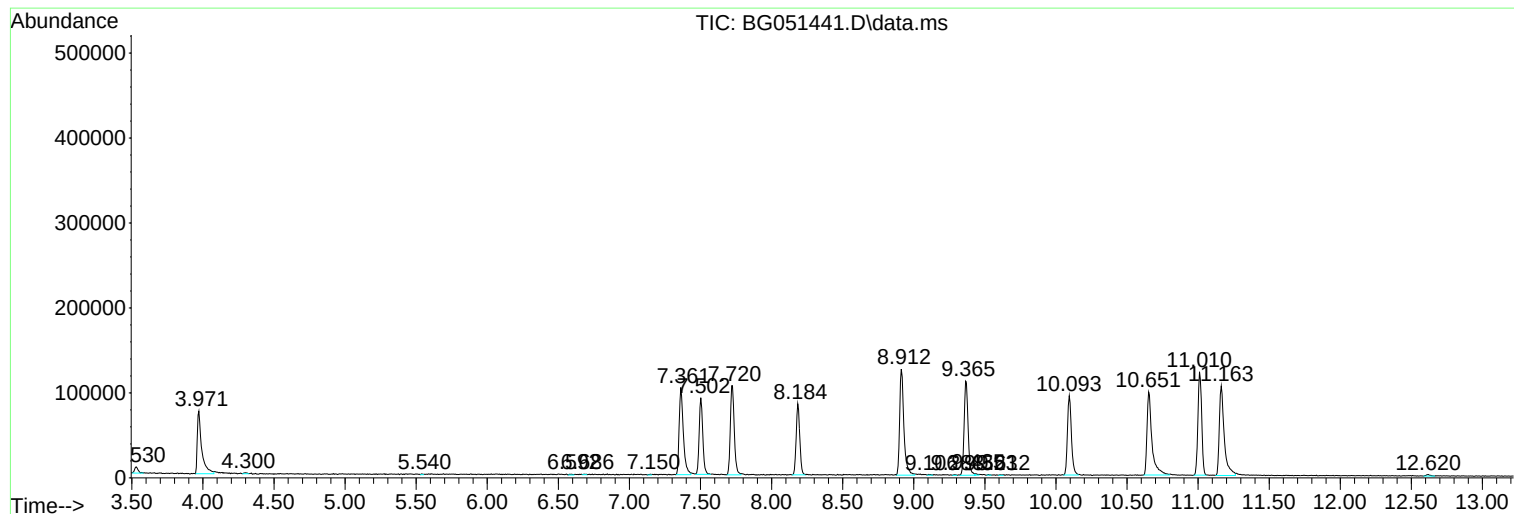

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
Data File : BG051441.D
Acq On : 9 Dec 2021 21:29
Operator : CG/JU
Sample : PB141217BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK217

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
Data File : BG051441.D
Acq On : 9 Dec 2021 21:29
Operator : CG/JU
Sample : PB141217BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK217

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------