

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
 Data File : BG051442.D
 Acq On : 9 Dec 2021 22:10
 Operator : CG/JU
 Sample : PB141181TB 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLEB181

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051442.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.529	3	7	15	rVB	9051	13378	1.51%	0.152%
2	3.969	78	82	105	rBV	80867	173369	19.51%	1.973%
3	4.163	113	115	117	rBV2	854	993	0.11%	0.011%
4	4.298	134	138	142	rBV5	1857	2695	0.30%	0.031%
5	4.927	244	245	248	rBV2	1085	894	0.10%	0.010%
6	5.691	373	375	379	rVB3	941	1234	0.14%	0.014%
7	5.720	379	380	383	rBV	810	931	0.10%	0.011%
8	6.349	483	487	491	rVB3	1031	1785	0.20%	0.020%
9	7.360	653	659	672	rBV	112434	230667	25.96%	2.625%
10	7.501	677	683	695	rVB	100183	177184	19.94%	2.016%
11	7.724	714	721	734	rVB	118373	223283	25.13%	2.541%
12	8.112	785	787	790	rBV2	736	1011	0.11%	0.012%
13	8.182	793	799	809	rVV	93444	167402	18.84%	1.905%
14	8.382	830	833	838	rBV2	717	1003	0.11%	0.011%
15	8.911	917	923	943	rBV	137881	286257	32.22%	3.257%
16	9.116	956	958	964	rVB	733	1294	0.15%	0.015%
17	9.369	994	1001	1015	rBV	124316	241049	27.13%	2.743%
18	9.733	1060	1063	1066	rBV2	991	1414	0.16%	0.016%
19	10.092	1118	1124	1137	rBV	102340	203921	22.95%	2.320%
20	10.203	1141	1143	1148	rVB	932	1131	0.13%	0.013%
21	10.650	1213	1219	1243	rBV	112194	272127	30.63%	3.097%
22	11.008	1273	1280	1289	rVB	137080	254548	28.65%	2.897%
23	11.161	1300	1306	1334	rBV	122190	280854	31.61%	3.196%
24	12.618	1549	1554	1558	rBV3	1333	2358	0.27%	0.027%
25	12.935	1606	1608	1613	rVB2	661	891	0.10%	0.010%
26	14.216	1819	1826	1840	rBV	286515	463673	52.18%	5.276%
27	14.516	1870	1877	1886	rBV	340744	545885	61.44%	6.212%
28	14.816	1922	1928	1937	rBV	227292	368246	41.44%	4.190%
29	15.086	1969	1974	2001	rBV2	44636	166639	18.75%	1.896%
30	15.297	2009	2010	2015	rVB4	1400	1426	0.16%	0.016%
31	15.808	2090	2097	2106	rBV	425731	677906	76.30%	7.714%
32	15.950	2116	2121	2133	rBV	93756	181124	20.38%	2.061%
33	16.032	2133	2135	2137	rVV3	3541	4066	0.46%	0.046%
34	16.049	2137	2138	2144	rVB4	2691	3460	0.39%	0.039%
35	17.354	2358	2360	2364	rBV2	974	1370	0.15%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
 Data File : BG051442.D
 Acq On : 9 Dec 2021 22:10
 Operator : CG/JU
 Sample : PB141181TB 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLEB181

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
 Title : SVOA CALIBRATION

36	17.565	2389	2396	2405	rBV	290397	463965	52.22%	5.279%
37	17.671	2407	2414	2429	rVB	458965	763661	85.95%	8.690%
38	18.229	2506	2509	2512	rVB3	630	911	0.10%	0.010%
39	19.346	2698	2699	2702	rBV3	1163	1102	0.12%	0.013%
40	19.440	2712	2715	2716	rBV3	985	1094	0.12%	0.012%
41	19.516	2722	2728	2732	rBV4	6859	9956	1.12%	0.113%
42	19.586	2737	2740	2749	rVB	6156	10460	1.18%	0.119%
43	19.663	2749	2753	2756	rBV4	1229	2499	0.28%	0.028%
44	19.704	2758	2760	2762	rVB2	1336	1027	0.12%	0.012%
45	19.827	2777	2781	2785	rVV7	1836	3269	0.37%	0.037%
46	19.898	2791	2793	2795	rBV3	1143	1020	0.11%	0.012%
47	19.951	2795	2802	2813	rVV	572161	888520	100.00%	10.110%
48	20.074	2821	2823	2825	rBV3	1638	1536	0.17%	0.017%
49	20.344	2867	2869	2872	rBV4	1680	2096	0.24%	0.024%
50	20.374	2872	2874	2876	rVV3	1777	1666	0.19%	0.019%
51	21.872	3122	3129	3139	rBV	246126	471255	53.04%	5.362%
52	25.027	3656	3666	3681	rBV2	249160	771451	86.82%	8.778%
53	25.268	3697	3707	3723	rVB4	132338	437144	49.20%	4.974%




Sum of corrected areas: 8788100

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
Data File : BG051442.D
Acq On : 9 Dec 2021 22:10
Operator : CG/JU
Sample : PB141181TB 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLEB181

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

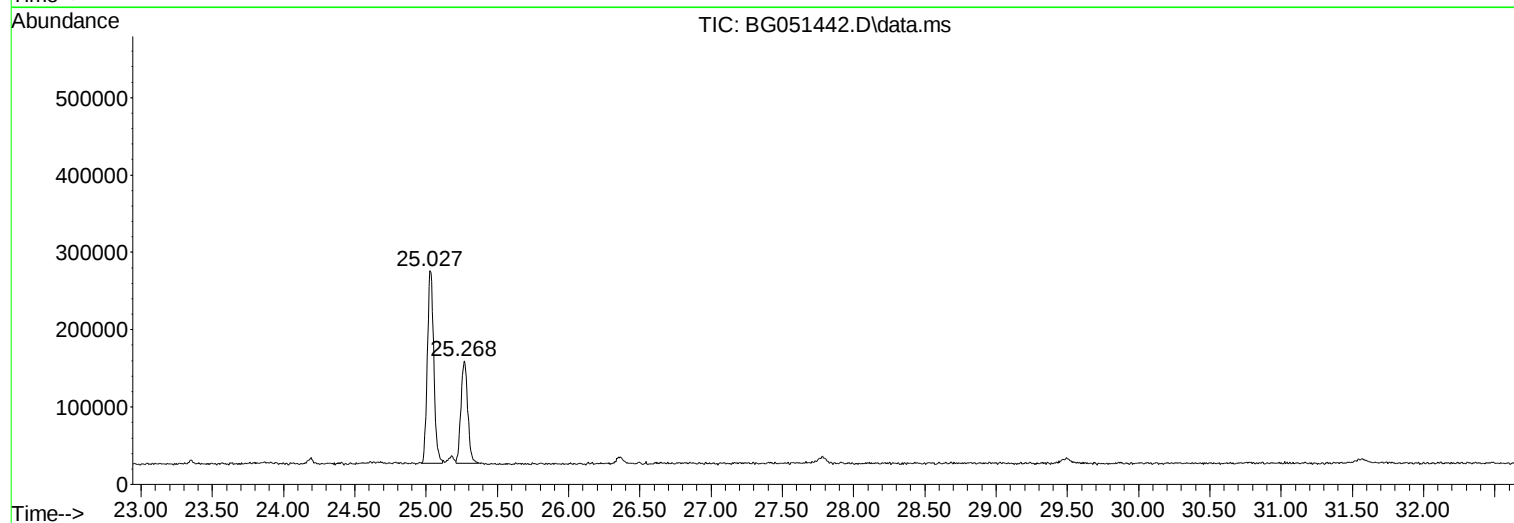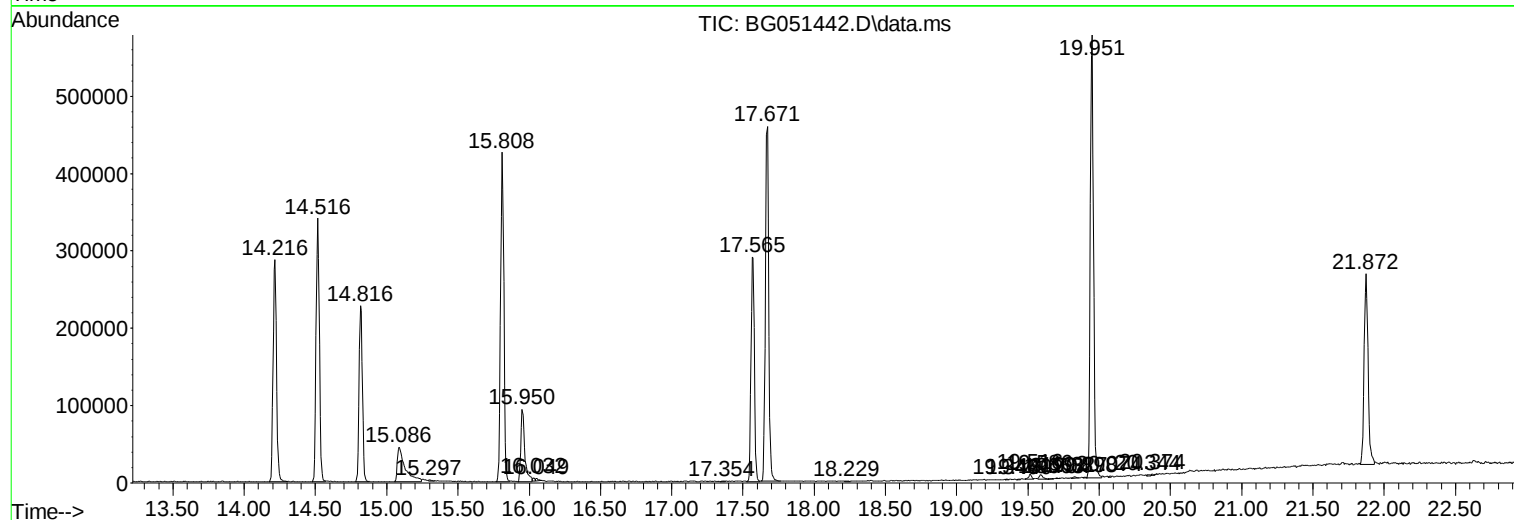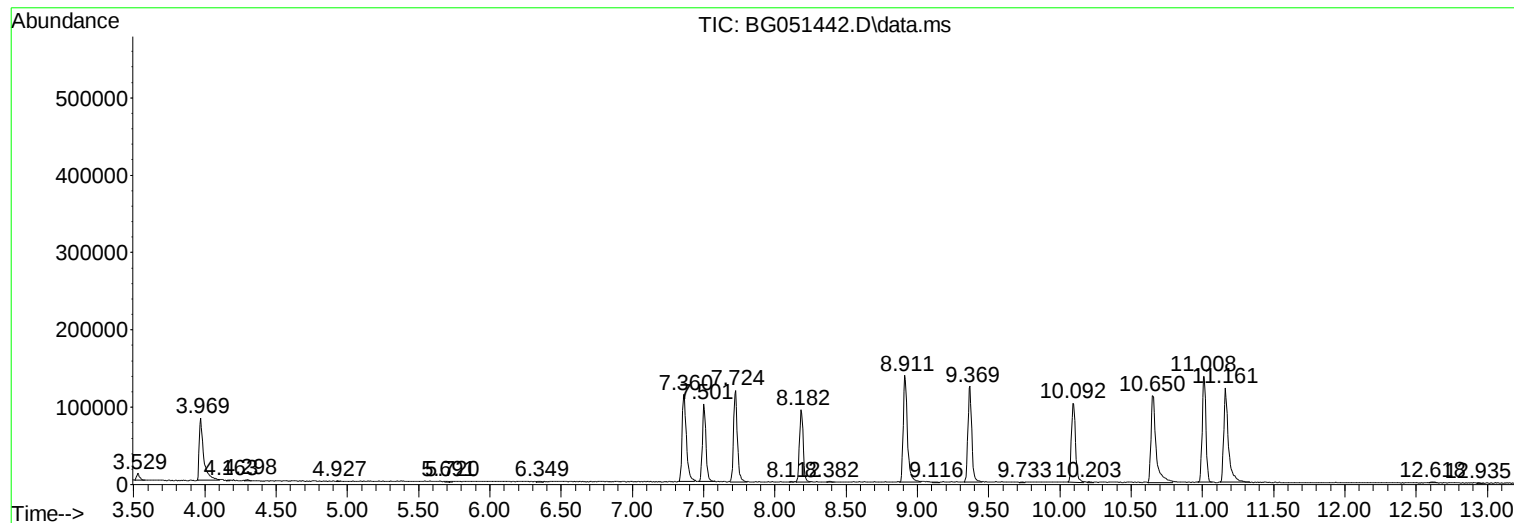

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
Data File : BG051442.D
Acq On : 9 Dec 2021 22:10
Operator : CG/JU
Sample : PB141181TB 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLEB181

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected
