

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
 Data File : BG051454.D
 Acq On : 10 Dec 2021 13:31
 Operator : CG/JU
 Sample : PB141293BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK293

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051454.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.528	3	7	13	rBV2	7413	12088	1.41%	0.149%
2	3.810	53	55	58	rVB3	950	940	0.11%	0.012%
3	3.975	78	83	99	rBV	71458	162963	19.07%	2.003%
4	4.298	134	138	144	rVB	7245	10902	1.28%	0.134%
5	4.604	187	190	192	rBV3	1147	1091	0.13%	0.013%
6	5.097	272	274	279	rVB	1068	940	0.11%	0.012%
7	5.226	293	296	298	rBV2	687	1037	0.12%	0.013%
8	5.279	302	305	309	rVB3	781	1324	0.15%	0.016%
9	5.367	316	320	321	rBV	988	865	0.10%	0.011%
10	5.602	359	360	365	rBV2	764	1106	0.13%	0.014%
11	6.378	490	492	494	rBV2	846	876	0.10%	0.011%
12	6.584	524	527	529	rBV2	819	1081	0.13%	0.013%
13	7.365	654	660	678	rBV	106605	225062	26.34%	2.766%
14	7.506	678	684	695	rVB	93016	167166	19.56%	2.055%
15	7.723	715	721	734	rBV	113211	211412	24.74%	2.598%
16	8.188	793	800	812	rVB	83027	152123	17.80%	1.870%
17	8.346	825	827	830	rBV2	749	858	0.10%	0.011%
18	8.916	918	924	938	rBV	123440	262512	30.72%	3.226%
19	9.151	962	964	969	rBV	577	931	0.11%	0.011%
20	9.369	994	1001	1013	rBV	119291	224944	26.33%	2.765%
21	9.609	1038	1042	1043	rBV	771	877	0.10%	0.011%
22	9.862	1082	1085	1087	rVB	938	1051	0.12%	0.013%
23	9.897	1087	1091	1092	rBV2	874	1123	0.13%	0.014%
24	10.097	1118	1125	1140	rVV	93876	189526	22.18%	2.329%
25	10.520	1194	1197	1199	rBV	929	1055	0.12%	0.013%
26	10.655	1214	1220	1236	rBV	98807	238409	27.90%	2.930%
27	11.014	1273	1281	1291	rVB	123867	229790	26.89%	2.824%
28	11.166	1301	1307	1326	rBV	98989	252963	29.61%	3.109%
29	12.618	1550	1554	1557	rBV2	1834	3044	0.36%	0.037%
30	14.216	1819	1826	1839	rBV	255097	423229	49.53%	5.202%
31	14.515	1870	1877	1890	rVB	309522	511039	59.81%	6.281%
32	14.815	1921	1928	1938	rVB	203274	329254	38.54%	4.047%
33	15.097	1971	1976	1998	rBV4	34949	138159	16.17%	1.698%
34	15.309	2010	2012	2015	rVB3	1009	1051	0.12%	0.013%
35	15.344	2015	2018	2023	rVB5	1027	1884	0.22%	0.023%
36	15.808	2091	2097	2110	rVB	400056	629661	73.69%	7.739%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
 Data File : BG051454.D
 Acq On : 10 Dec 2021 13:31
 Operator : CG/JU
 Sample : PB141293BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK293

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
 Title : SVOA CALIBRATION

37	15.902	2112	2113	2117	rVB2	1100	1061	0.12%	0.013%
38	15.955	2117	2122	2134	rBV2	83182	164159	19.21%	2.018%
39	16.266	2172	2175	2178	rVB2	1067	1354	0.16%	0.017%
40	16.531	2217	2220	2226	rVB3	608	1124	0.13%	0.014%
41	16.742	2253	2256	2260	rVB3	544	916	0.11%	0.011%
42	17.571	2390	2397	2407	rBV	262335	414446	48.51%	5.094%
43	17.671	2407	2414	2427	rVB	422967	701983	82.16%	8.628%
44	18.240	2507	2511	2513	rVB2	607	875	0.10%	0.011%
45	18.464	2544	2549	2551	rBV5	943	1426	0.17%	0.018%
46	18.534	2557	2561	2562	rBV3	1111	1188	0.14%	0.015%
47	18.816	2606	2609	2610	rVB2	1298	1097	0.13%	0.013%
48	18.846	2610	2614	2615	rBV	1232	1431	0.17%	0.018%
49	18.951	2628	2632	2633	rVB3	905	980	0.11%	0.012%
50	19.128	2657	2662	2663	rBV3	762	986	0.12%	0.012%
51	19.204	2673	2675	2679	rBV3	1559	1442	0.17%	0.018%
52	19.515	2724	2728	2734	rVB4	6036	8985	1.05%	0.110%
53	19.592	2736	2741	2747	rBV4	7062	11318	1.32%	0.139%
54	19.827	2778	2781	2787	rBV5	3995	6568	0.77%	0.081%
55	19.950	2796	2802	2816	rBV	538723	854416	100.00%	10.501%
56	20.320	2863	2865	2866	rBV2	1537	935	0.11%	0.011%
57	20.626	2910	2917	2918	rBV6	5707	9755	1.14%	0.120%
58	20.861	2954	2957	2961	rBV6	5760	6099	0.71%	0.075%
59	21.872	3123	3129	3140	rBV	215169	430754	50.42%	5.294%
60	24.416	3560	3562	3564	rBV3	3897	3948	0.46%	0.049%
61	25.027	3656	3666	3685	rBV2	227118	730866	85.54%	8.983%
62	25.268	3698	3707	3721	rVB2	122418	385996	45.18%	4.744%




Sum of corrected areas: 8136444

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
Data File : BG051454.D
Acq On : 10 Dec 2021 13:31
Operator : CG/JU
Sample : PB141293BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK293

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

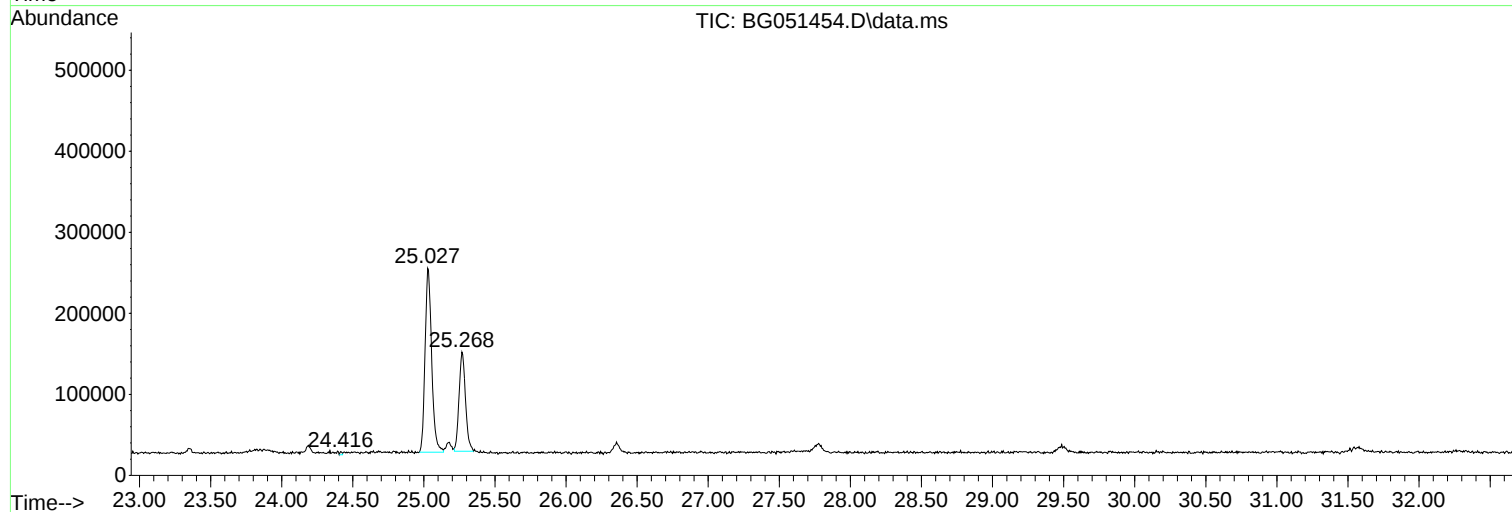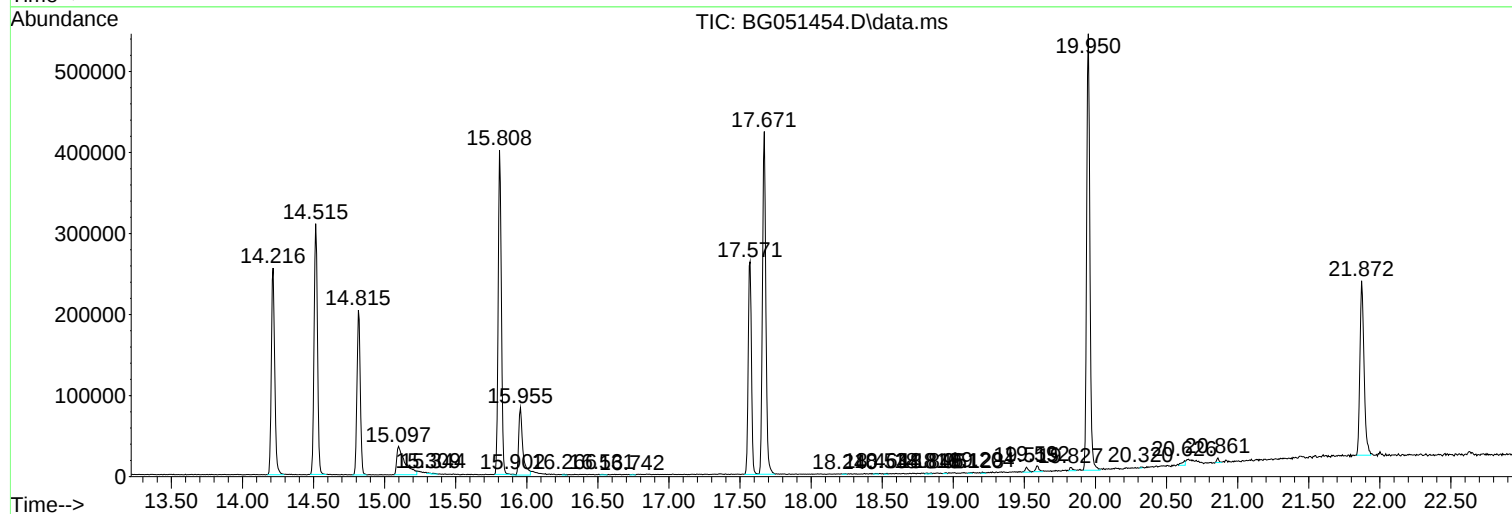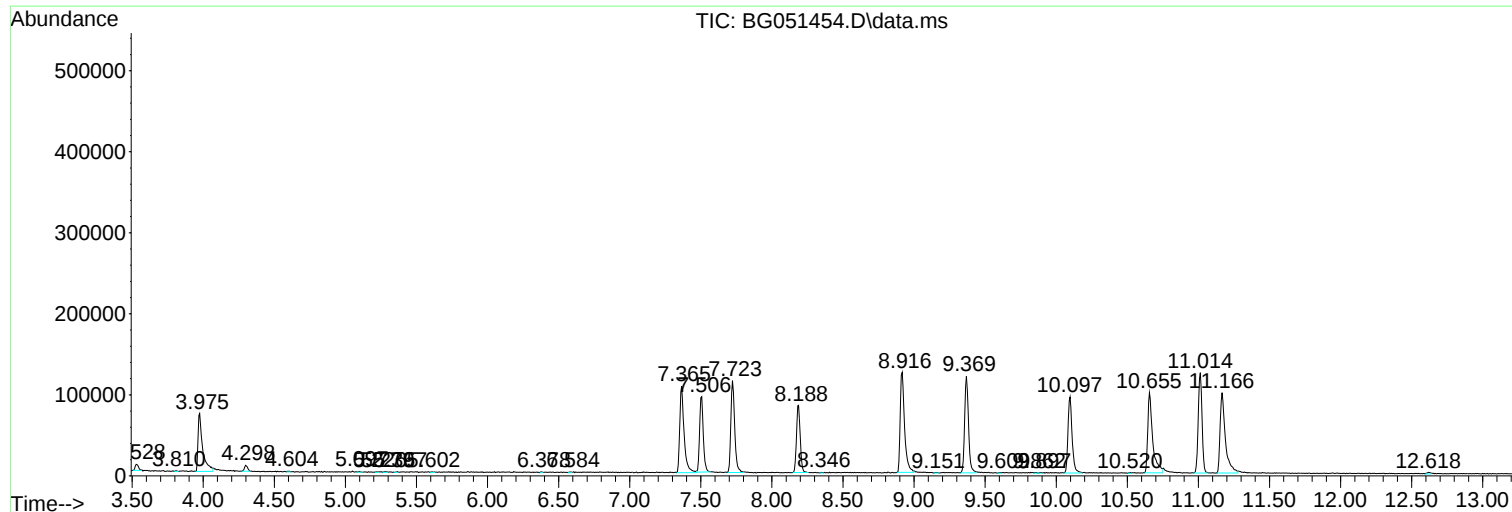

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
Data File : BG051454.D
Acq On : 10 Dec 2021 13:31
Operator : CG/JU
Sample : PB141293BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK293

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
Data File : BG051454.D
Acq On : 10 Dec 2021 13:31
Operator : CG/JU
Sample : PB141293BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK293

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc