

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
 Data File : BG051455.D
 Acq On : 10 Dec 2021 14:13
 Operator : CG/JU
 Sample : PB141295BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK295

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051455.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.535	3	8	16	rVB3	7723	14757	1.72%	0.183%
2	3.764	45	47	49	rBV3	944	1033	0.12%	0.013%
3	3.970	78	82	104	rBV	70789	161432	18.76%	2.001%
4	4.299	134	138	146	rVB3	7864	13111	1.52%	0.163%
5	4.610	189	191	194	rBV3	890	959	0.11%	0.012%
6	4.904	240	241	243	rBV	1001	896	0.10%	0.011%
7	5.039	262	264	267	rBV3	713	873	0.10%	0.011%
8	5.174	286	287	293	rVV4	844	1189	0.14%	0.015%
9	5.703	374	377	381	rBV2	667	984	0.11%	0.012%
10	6.150	451	453	456	rVB2	1033	974	0.11%	0.012%
11	6.244	467	469	472	rVB2	1166	1058	0.12%	0.013%
12	6.414	496	498	502	rVB2	800	1018	0.12%	0.013%
13	6.467	505	507	510	rVV2	1139	1017	0.12%	0.013%
14	6.538	517	519	523	rVB3	1041	1332	0.15%	0.017%
15	6.767	556	558	562	rVB2	1128	1171	0.14%	0.015%
16	6.814	562	566	568	rBV2	981	1422	0.17%	0.018%
17	7.366	654	660	675	rBV	99318	216044	25.11%	2.678%
18	7.501	677	683	694	rVV	91278	161175	18.73%	1.998%
19	7.724	715	721	736	rVB	107362	206762	24.03%	2.563%
20	7.824	736	738	742	rBV2	1098	1271	0.15%	0.016%
21	8.189	793	800	812	rBV	80591	147164	17.11%	1.824%
22	8.482	848	850	853	rBV2	868	913	0.11%	0.011%
23	8.917	917	924	940	rBV2	122624	256471	29.81%	3.179%
24	9.370	994	1001	1014	rBV2	113994	216356	25.15%	2.682%
25	9.710	1056	1059	1062	rBV2	720	1106	0.13%	0.014%
26	10.098	1118	1125	1141	rBV2	92870	184806	21.48%	2.291%
27	10.480	1187	1190	1193	rBV2	781	912	0.11%	0.011%
28	10.656	1214	1220	1244	rBV	93995	239874	27.88%	2.973%
29	10.827	1248	1249	1252	rVV	1193	893	0.10%	0.011%
30	11.015	1273	1281	1289	rBV	121537	224259	26.07%	2.780%
31	11.167	1300	1307	1324	rBV	96251	245664	28.55%	3.045%
32	12.625	1550	1555	1562	rVB2	1606	2962	0.34%	0.037%
33	14.217	1819	1826	1837	rBV	265423	421617	49.01%	5.226%
34	14.364	1848	1851	1854	rVB2	800	888	0.10%	0.011%
35	14.516	1871	1877	1890	rVB	312236	508758	59.14%	6.307%
36	14.822	1920	1929	1939	rBV	195675	322955	37.54%	4.003%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
 Data File : BG051455.D
 Acq On : 10 Dec 2021 14:13
 Operator : CG/JU
 Sample : PB141295BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK295

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
 Title : SVOA CALIBRATION

37	14.975	1951	1955	1959	rVB	599	881	0.10%	0.011%
38	15.098	1970	1976	1999	rBV4	35426	142566	16.57%	1.767%
39	15.304	2009	2011	2017	rVB5	1342	1639	0.19%	0.020%
40	15.586	2057	2059	2064	rBV2	990	1106	0.13%	0.014%
41	15.809	2090	2097	2107	rBV	389596	634329	73.73%	7.863%
42	15.956	2116	2122	2137	rBV	84557	168342	19.57%	2.087%
43	16.079	2142	2143	2146	rVB2	1106	960	0.11%	0.012%
44	17.072	2308	2312	2314	rBV2	603	889	0.10%	0.011%
45	17.366	2360	2362	2366	rVB	1209	1050	0.12%	0.013%
46	17.572	2389	2397	2405	rBV	260765	417067	48.48%	5.170%
47	17.672	2407	2414	2426	rVV	424509	712633	82.83%	8.834%
48	18.218	2504	2507	2510	rBV4	842	1278	0.15%	0.016%
49	18.788	2601	2604	2605	rBV2	987	1013	0.12%	0.013%
50	19.182	2669	2671	2676	rVB4	1343	1452	0.17%	0.018%
51	19.270	2684	2686	2690	rVV3	649	914	0.11%	0.011%
52	19.516	2724	2728	2735	rBV4	5961	9322	1.08%	0.116%
53	19.593	2737	2741	2746	rVV	7045	10423	1.21%	0.129%
54	19.828	2778	2781	2783	rBV4	4509	4536	0.53%	0.056%
55	19.887	2788	2791	2793	rBV4	1820	1871	0.22%	0.023%
56	19.951	2795	2802	2817	rVV	550439	860329	100.00%	10.665%
57	20.744	2935	2937	2938	rVB2	2876	1332	0.15%	0.017%
58	20.862	2954	2957	2959	rBV4	5091	4835	0.56%	0.060%
59	21.873	3123	3129	3142	rVB	212401	426554	49.58%	5.288%
60	25.034	3657	3667	3682	rBV2	231057	705929	82.05%	8.751%
61	25.269	3698	3707	3723	rVB2	123854	391863	45.55%	4.857%




Sum of corrected areas: 8067189

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
Data File : BG051455.D
Acq On : 10 Dec 2021 14:13
Operator : CG/JU
Sample : PB141295BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK295

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

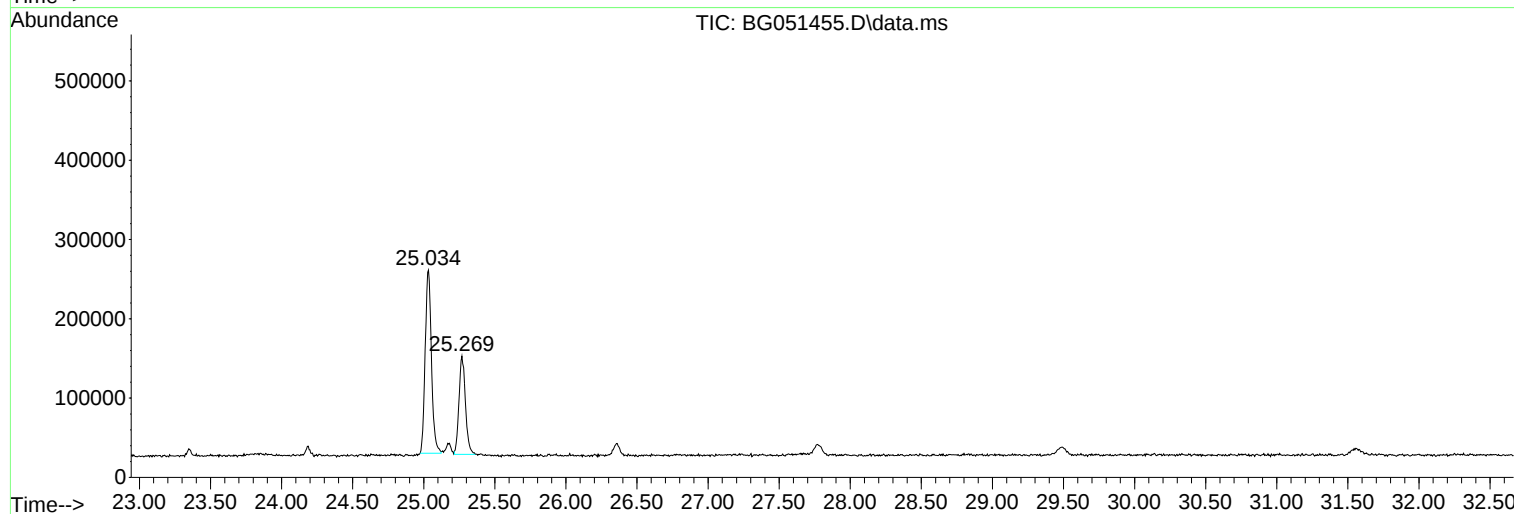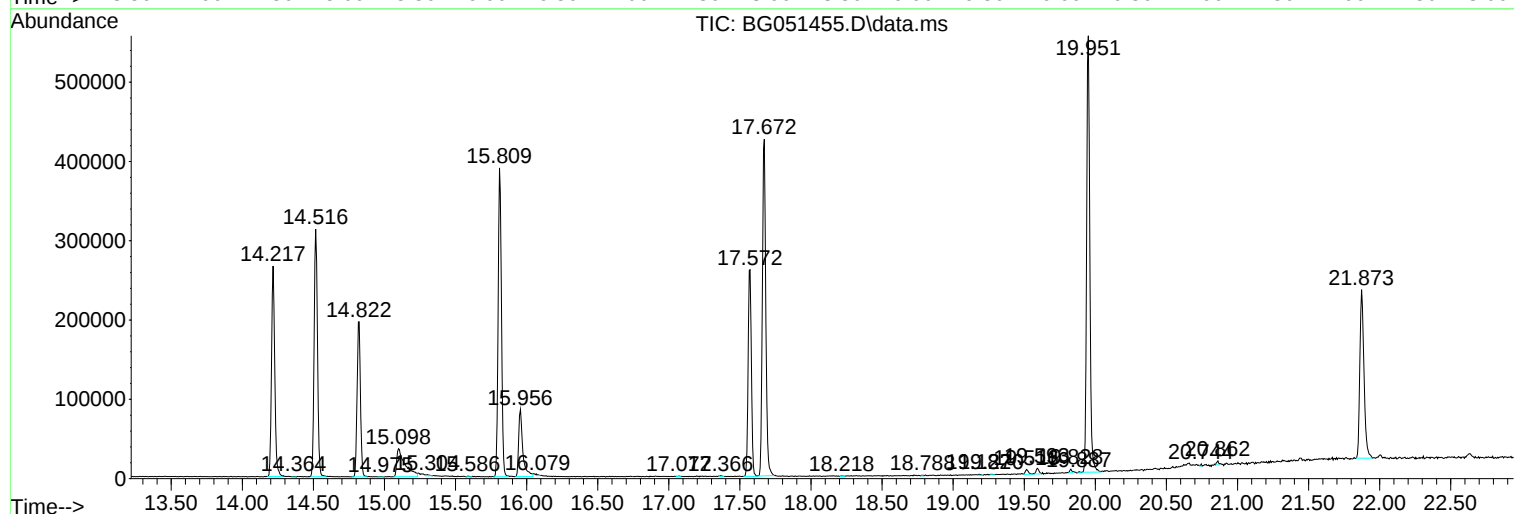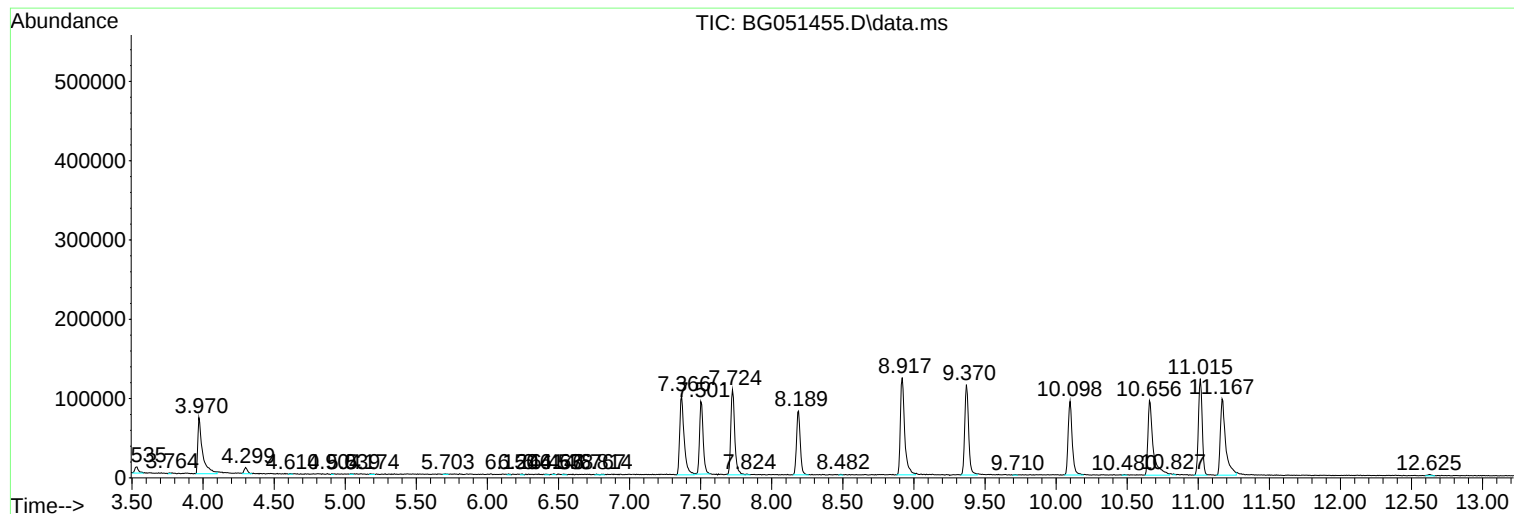

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
Data File : BG051455.D
Acq On : 10 Dec 2021 14:13
Operator : CG/JU
Sample : PB141295BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK295

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120921\
Data File : BG051455.D
Acq On : 10 Dec 2021 14:13
Operator : CG/JU
Sample : PB141295BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK295

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc