


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120922\
 Data File : BG055940.D
 Acq On : 9 Dec 2022 10:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 09 07:57:14 2022

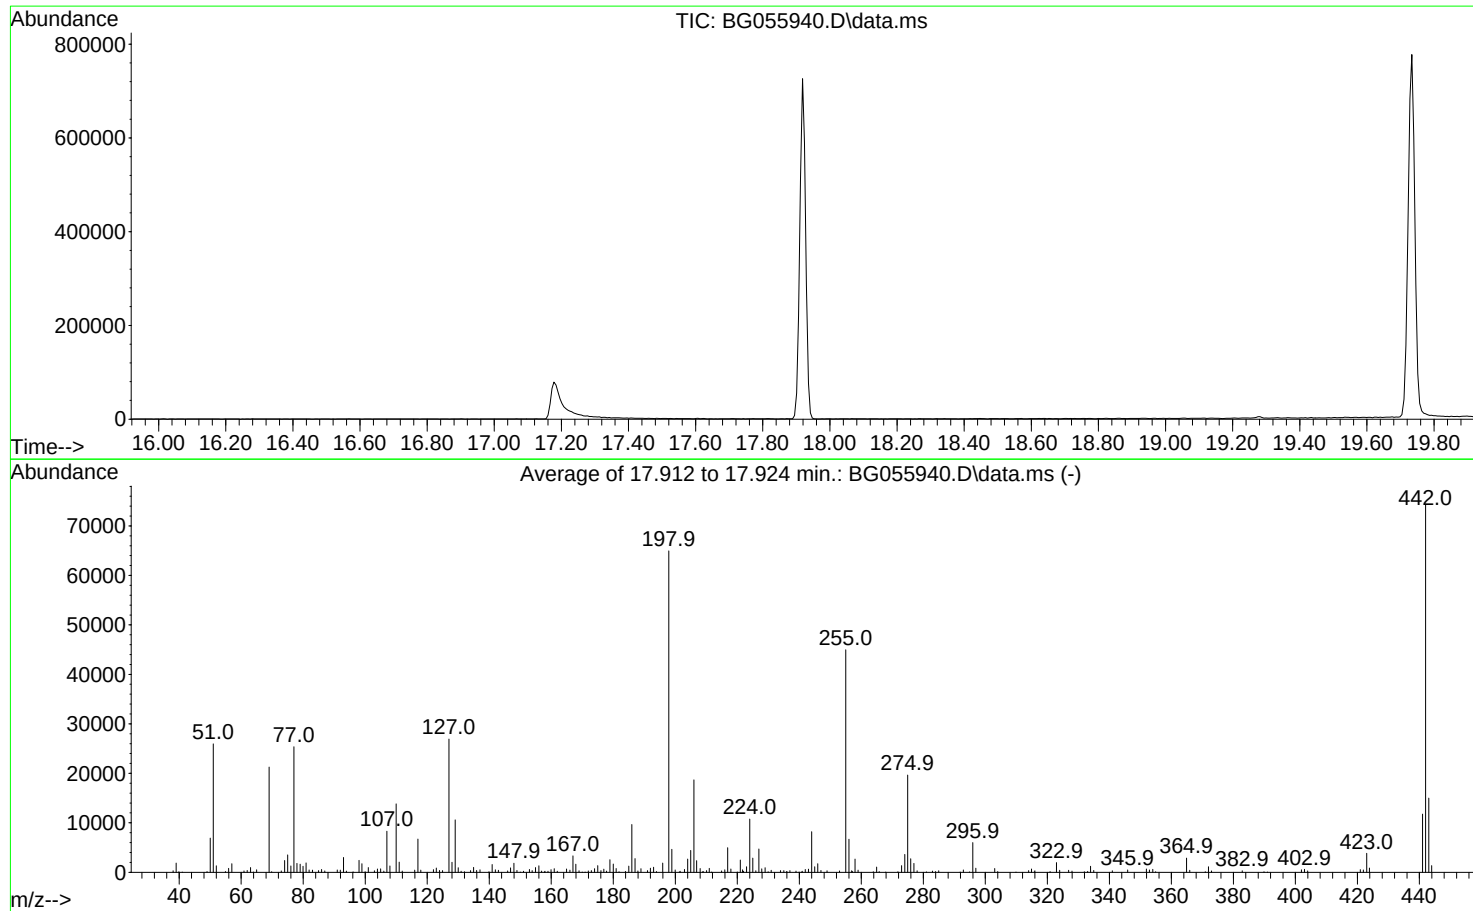




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	25971	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.7	21253	PASS
70	69	0.00	2	0.6	126	PASS
127	198	10	80	41.5	26925	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64952	PASS
199	198	5	9	7.2	4653	PASS
275	198	10	60	30.2	19644	PASS
365	198	1	100	4.4	2876	PASS
441	198	0.01	100	18.1	11768	PASS
442	442	50	100	100.0	74347	PASS
443	442	15	24	20.2	14994	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120922\
Data File : BG055940.D
Acq On : 9 Dec 2022 10:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 10 07:51:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 09 07:57:14 2022
Response via : Initial Calibration

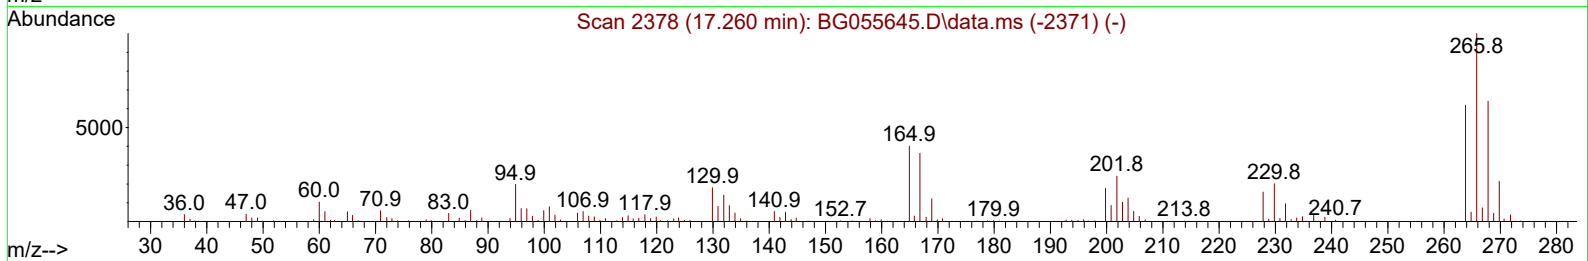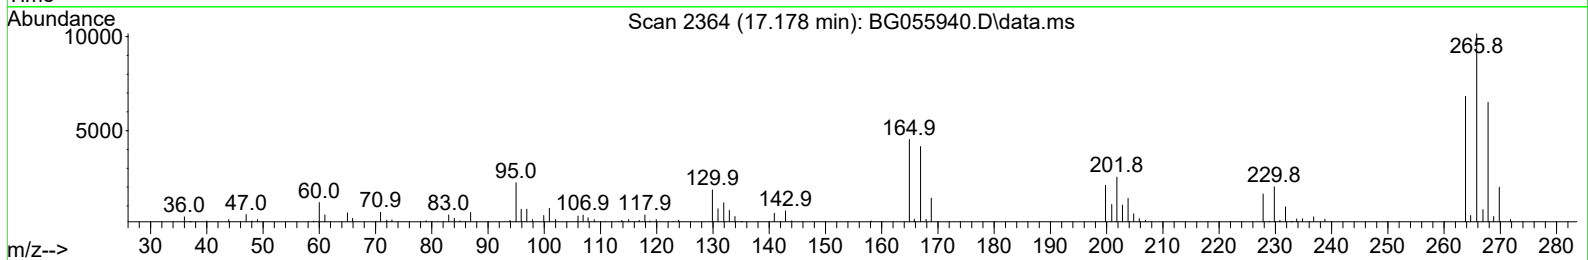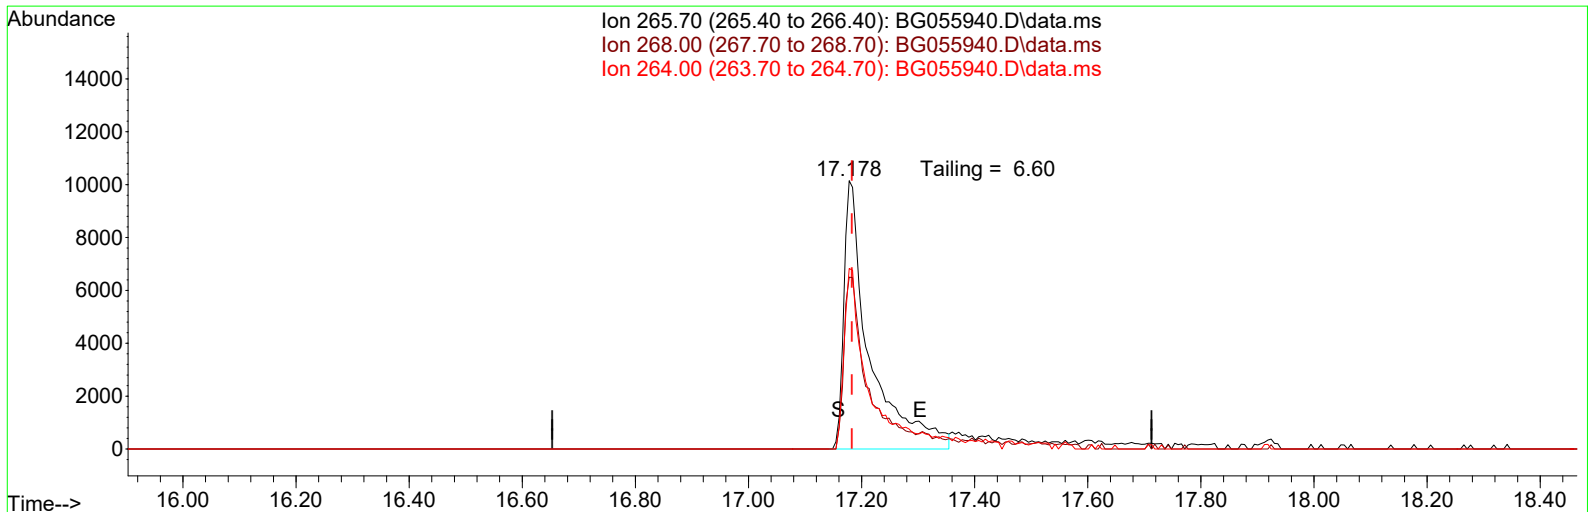

TIC: BG055940.D\data.ms

(70) Pentachlorophenol (C)

17.178min (-0.005) 12391.26 ng




response 29113

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.01
264.00	61.90	72.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120922\
Data File : BG055940.D
Acq On : 9 Dec 2022 10:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 10 07:51:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 09 07:57:14 2022
Response via : Initial Calibration

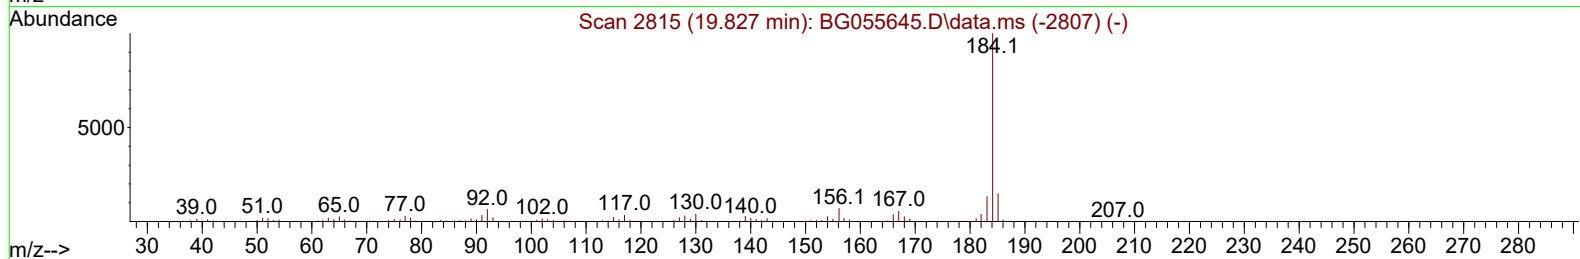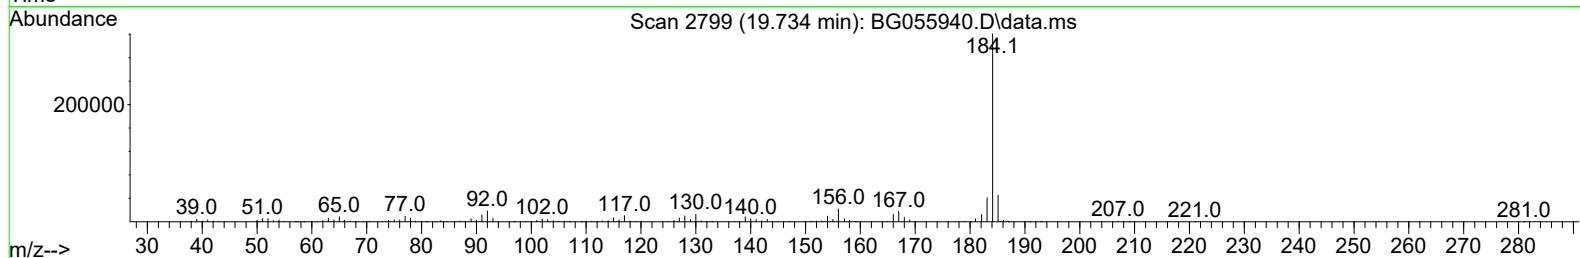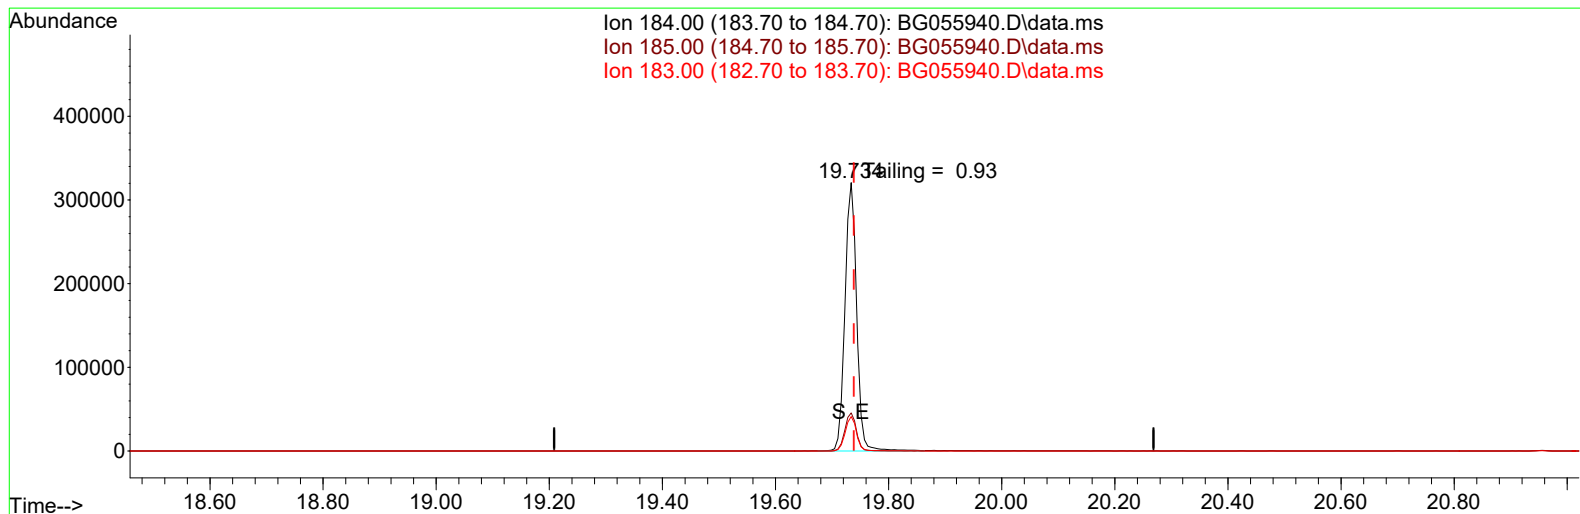

TIC: BG055940.D\data.ms

(77) Benzidine

19.734min (-0.005) 0.00 ng

response 460727

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.21
183.00	13.20	12.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/9/2022	BNA_G	BG055940.D
Compound Name	Response	Retention Time
DDT	205598	20.956
DDD	5368	20.562
DDE	444	20.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5812	211410	2.75

Instrument :
BNA_G
ClientSampleId :
DFTPP