
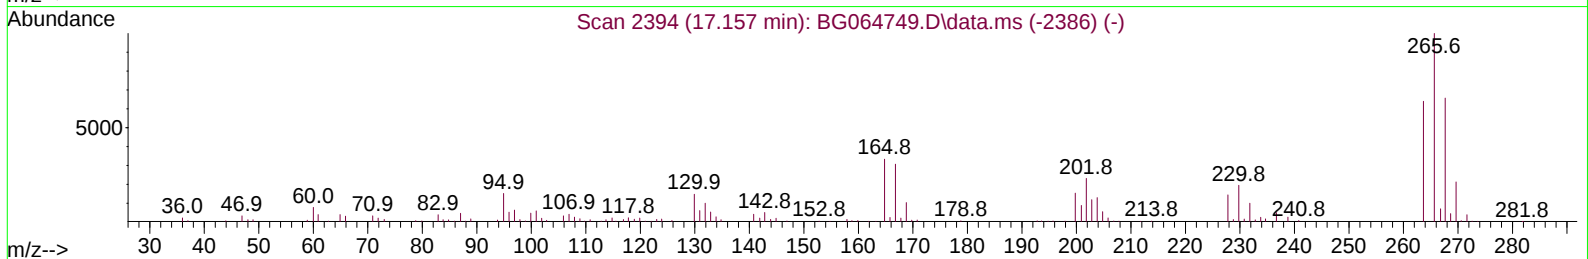
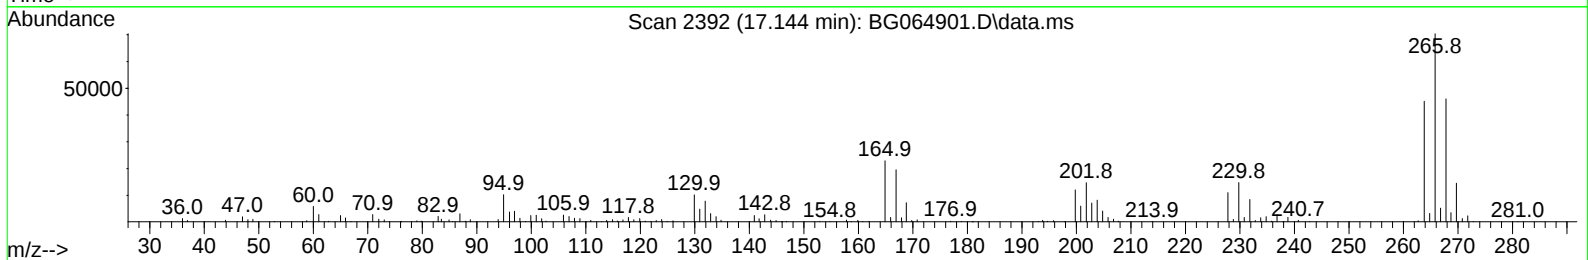


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120925\
Data File : BG064901.D
Acq On : 9 Dec 2025 11:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 12:18:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

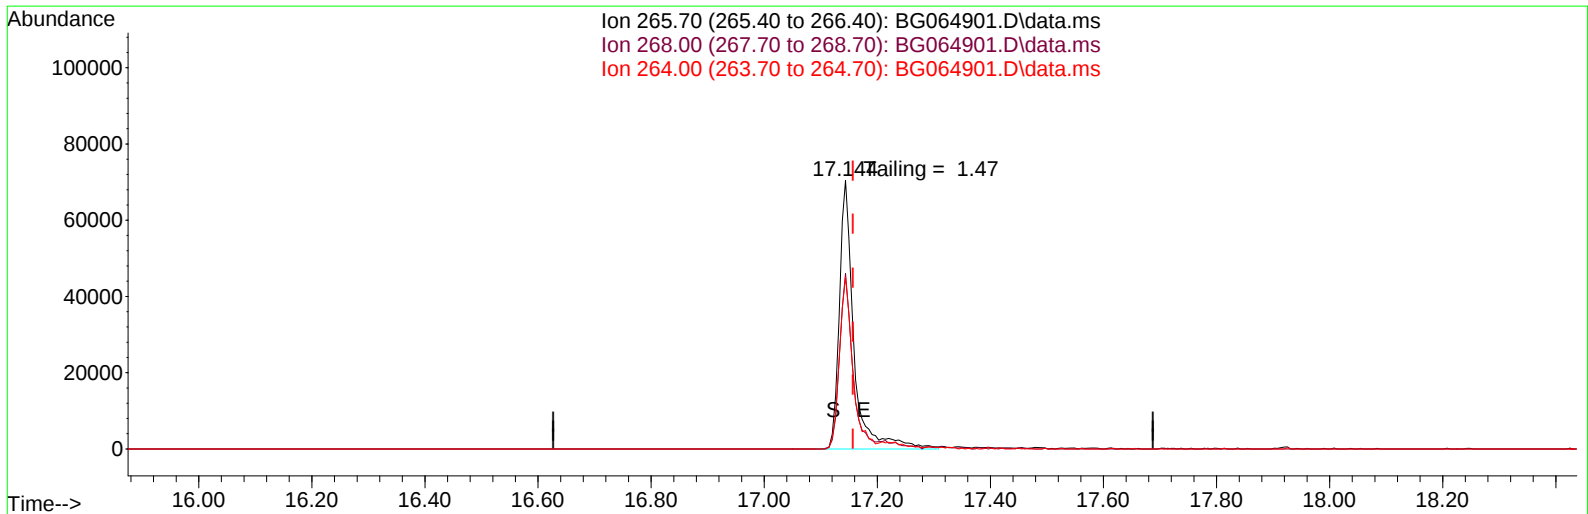

TIC: BG064901.D\data.ms

(70) Pentachlorophenol (C)




17.144min (-0.013) 25114.17 ng

response 118300

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.10	70.42
264.00	64.00	64.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120925\
Data File : BG064901.D
Acq On : 9 Dec 2025 11:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 12:18:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

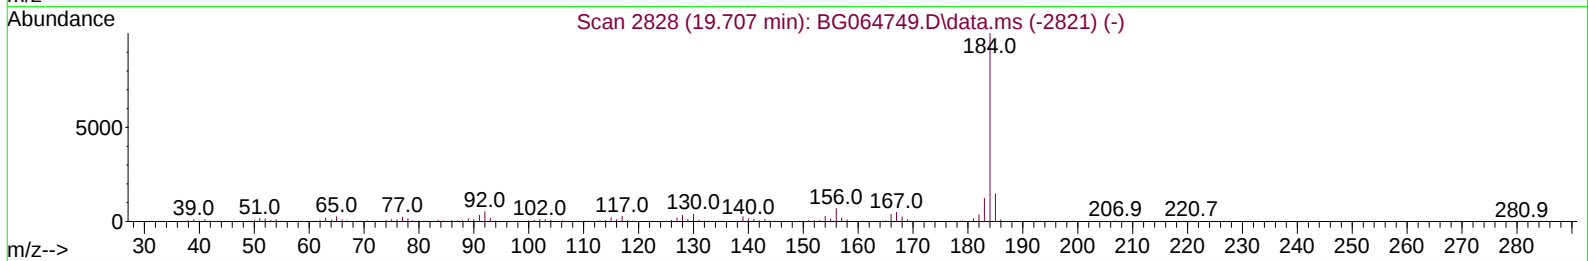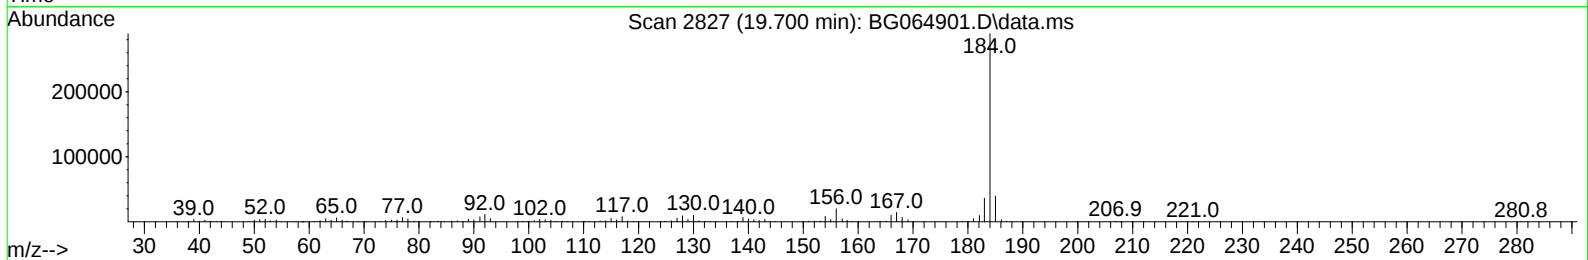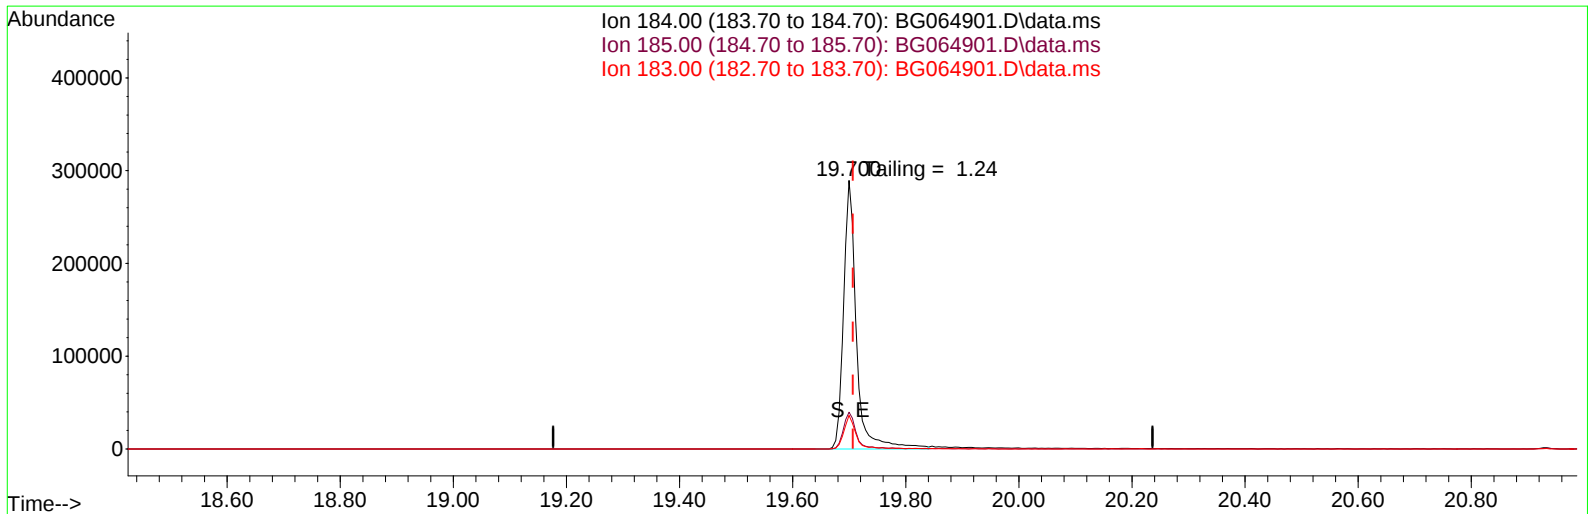

TIC: BG064901.D\data.ms

(77) Benzidine

19.700min (-0.007) 0.00 ng

response 454693

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.70
183.00	12.20	12.52
0.00	0.00	0.00