
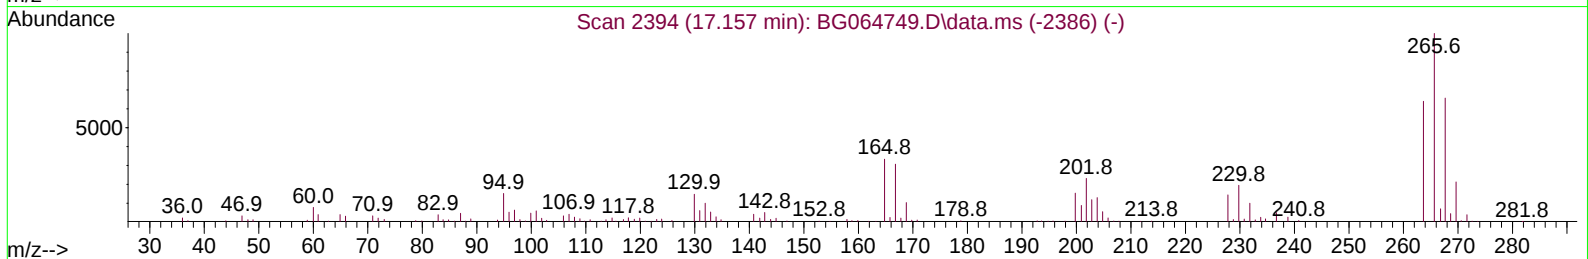
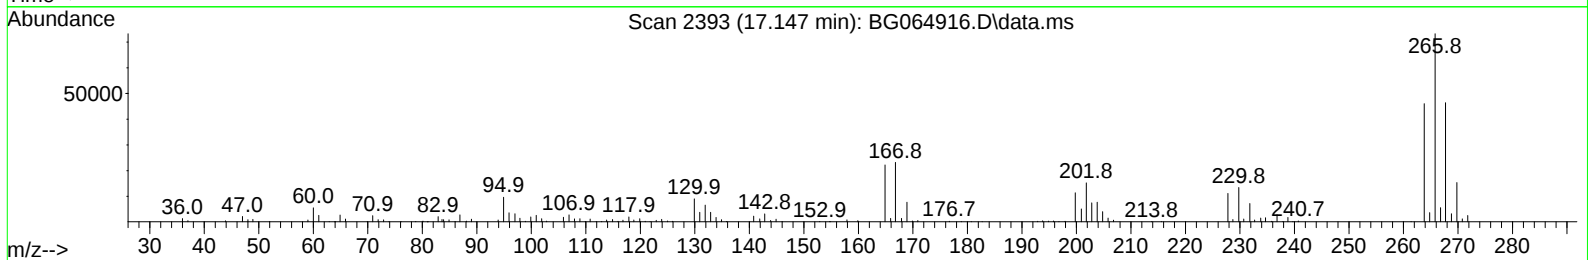


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121025\
Data File : BG064916.D
Acq On : 10 Dec 2025 10:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 11:23:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

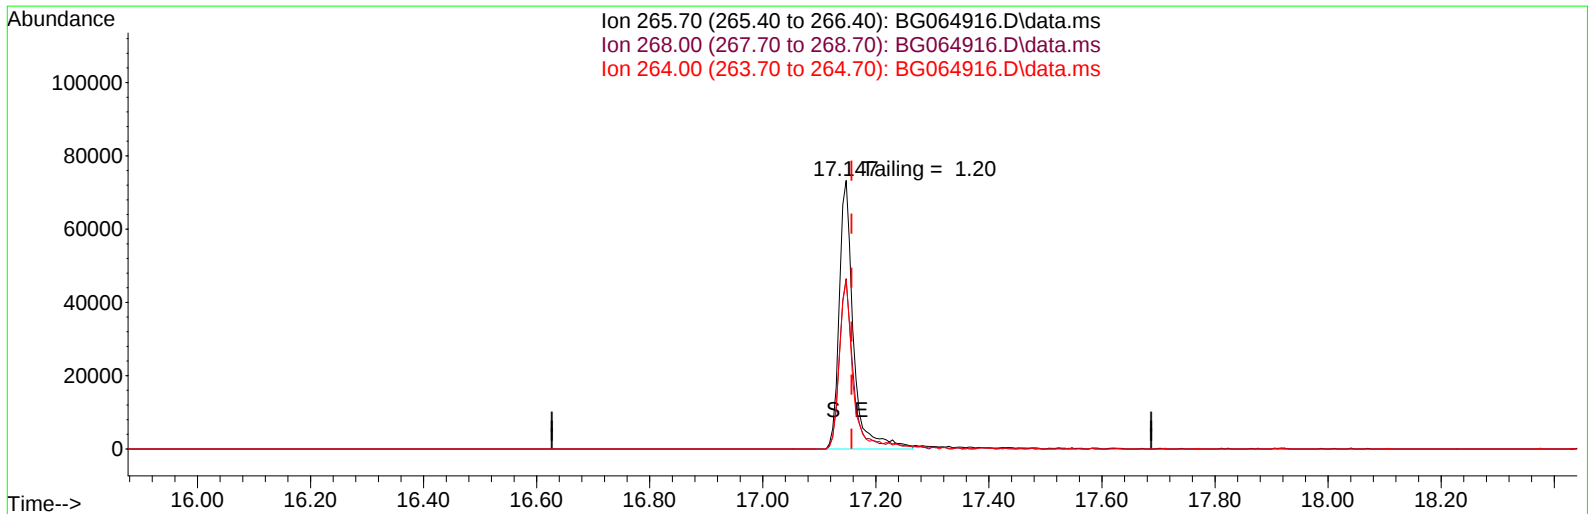

TIC: BG064916.D\data.ms

(70) Pentachlorophenol (C)




17.147min (-0.010) 29506.23 ng

response 128464

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.10	63.40
264.00	64.00	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121025\
Data File : BG064916.D
Acq On : 10 Dec 2025 10:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 11:23:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

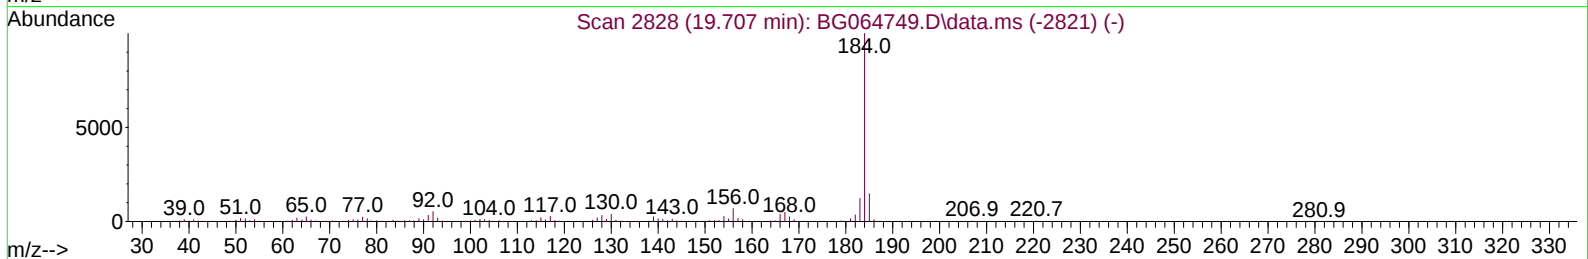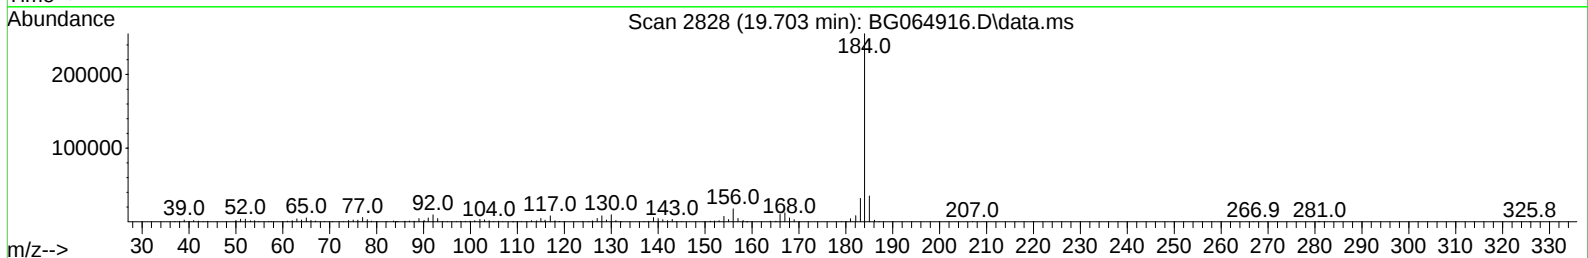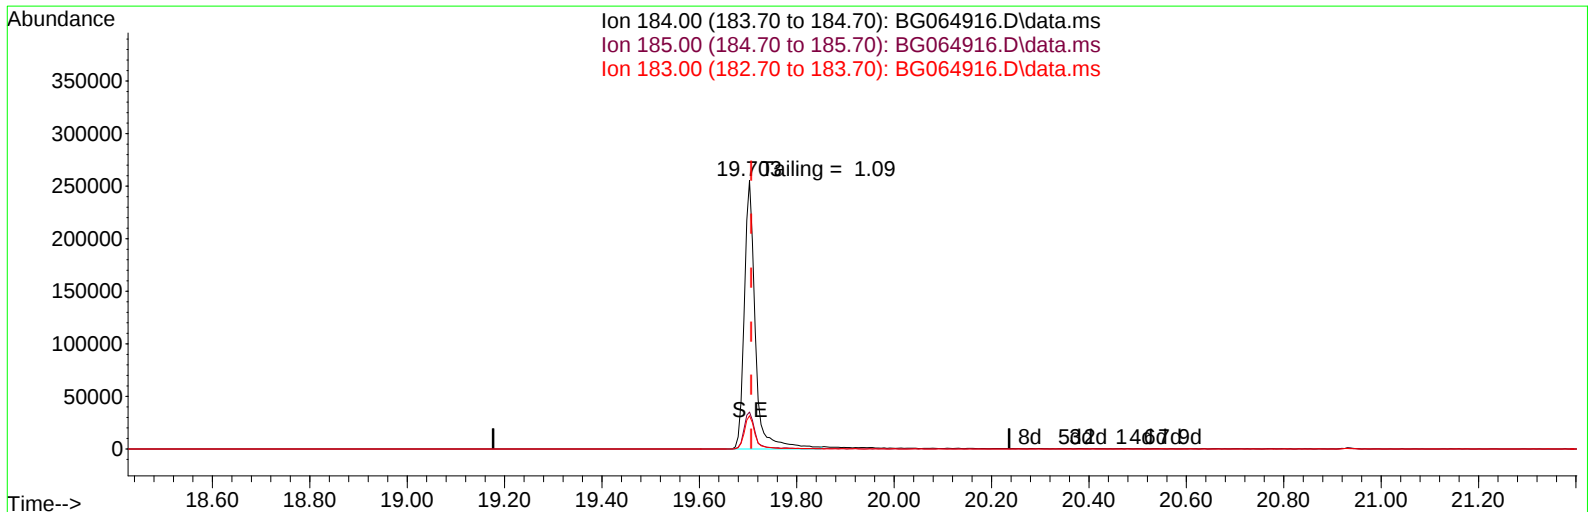

TIC: BG064916.D\data.ms

(77) Benzidine**19.703min (-0.004) 218453.11 ng m****response 425251**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.76
183.00	12.20	12.40
0.00	0.00	0.00