

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121025\
Data File : BG064918.D
Acq On : 10 Dec 2025 12:58
Operator : RC/JU
Sample : PB170885BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB170885BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG064918.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.203	354	360	367	rBV	90078	134032	4.71%	1.454%
2	5.684	435	442	456	rBV	348026	578128	20.32%	6.270%
3	7.294	709	716	725	rBV	336770	592632	20.83%	6.427%
4	8.146	854	861	870	rBV	77382	132464	4.66%	1.437%
5	9.309	1052	1059	1070	rBV2	193514	375579	13.20%	4.073%
6	10.966	1334	1341	1358	rBV	90135	185057	6.50%	2.007%
7	13.393	1747	1754	1762	rBV	672806	1093988	38.45%	11.864%
8	14.768	1980	1988	2000	rBV	182023	310056	10.90%	3.363%
9	16.243	2232	2239	2256	rBV2	724200	1208922	42.49%	13.111%
10	17.494	2446	2452	2464	rBV2	270346	450324	15.83%	4.884%
11	20.085	2887	2893	2909	rBV	2113756	2845148	100.00%	30.855%
12	21.748	3169	3176	3190	rBV	351626	641199	22.54%	6.954%
13	25.009	3720	3731	3743	rBV	222447	673375	23.67%	7.303%




Sum of corrected areas: 9220904

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121025\
Data File : BG064918.D
Acq On : 10 Dec 2025 12:58
Operator : RC/JU
Sample : PB170885BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB170885BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

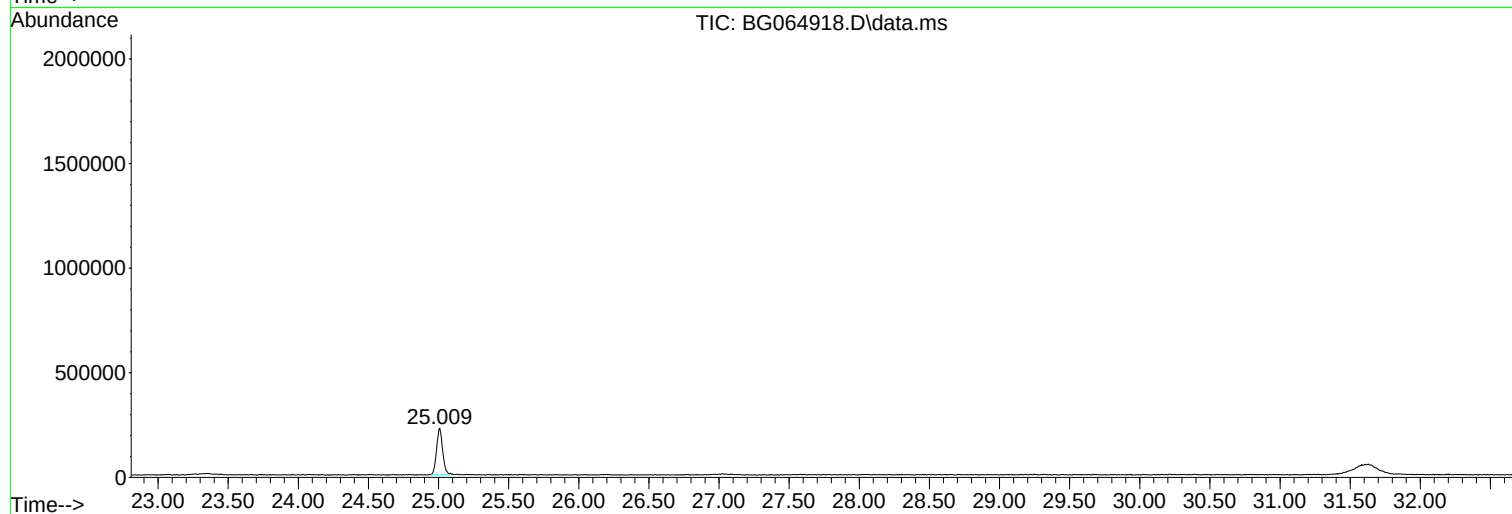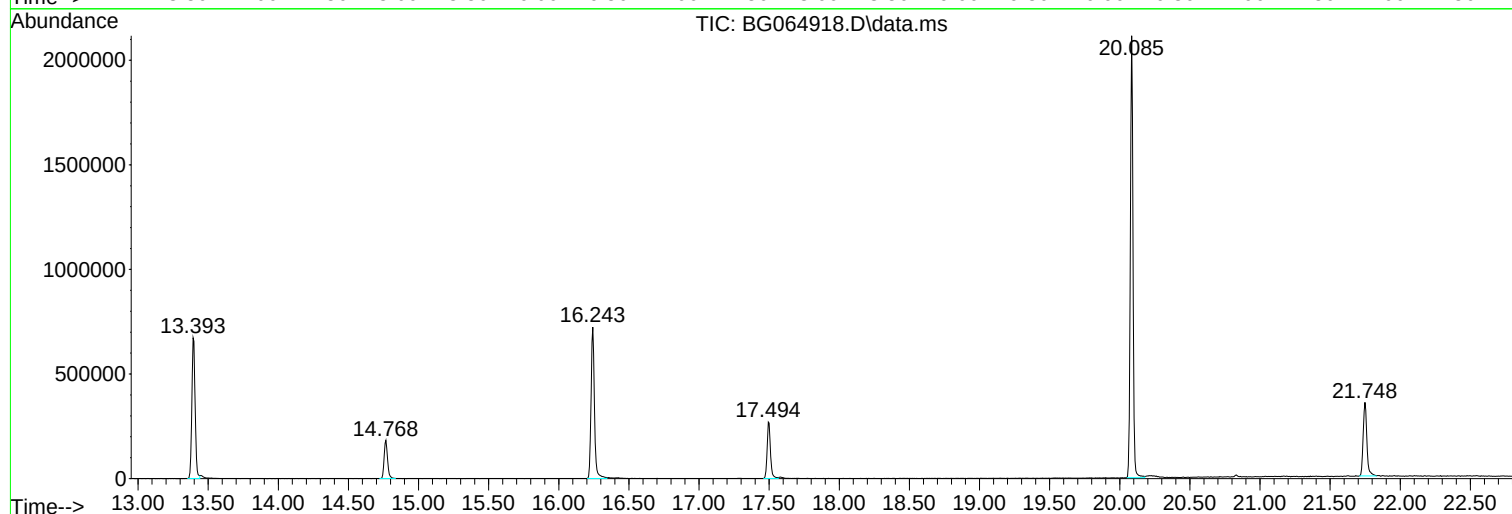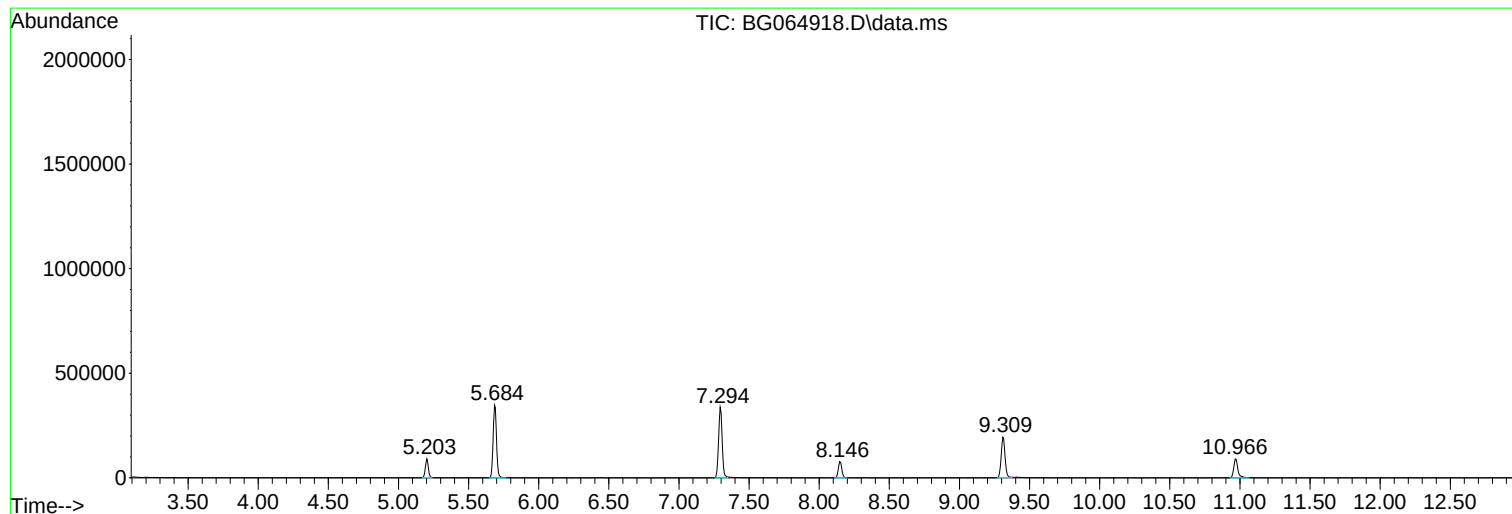

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121025\
Data File : BG064918.D
Acq On : 10 Dec 2025 12:58
Operator : RC/JU
Sample : PB170885BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB170885BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121025\
Data File : BG064918.D
Acq On : 10 Dec 2025 12:58
Operator : RC/JU
Sample : PB170885BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB170885BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------