

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121025\
 Data File : BG064925.D
 Acq On : 10 Dec 2025 17:51
 Operator : RC/JU
 Sample : Q3814-11
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-12

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG064925.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.120	3	5	15	rVB4	10599	20255	1.11%	0.168%
2	3.202	15	19	33	rVB	30770	51184	2.80%	0.425%
3	5.206	354	360	368	rBV	55715	85608	4.68%	0.710%
4	5.688	436	442	456	rBV	205036	339358	18.55%	2.815%
5	7.298	709	716	727	rBV	191165	347097	18.98%	2.879%
6	8.149	856	861	868	rBV	56938	96163	5.26%	0.798%
7	9.313	1052	1059	1069	rBV	118340	219790	12.02%	1.823%
8	10.970	1333	1341	1352	rBV	66663	129074	7.06%	1.071%
9	13.396	1747	1754	1765	rBV	376029	617537	33.76%	5.123%
10	13.790	1817	1821	1827	rVB4	23787	34387	1.88%	0.285%
11	13.931	1839	1845	1849	rBV2	41854	66931	3.66%	0.555%
12	14.054	1860	1866	1870	rBV2	162398	249374	13.63%	2.069%
13	14.095	1870	1873	1881	rVB2	112524	176668	9.66%	1.466%
14	14.207	1884	1892	1896	rBV2	20807	40230	2.20%	0.334%
15	14.301	1902	1908	1913	rVB2	53308	81141	4.44%	0.673%
16	14.765	1981	1987	1996	rBV	136030	237555	12.99%	1.971%
17	15.018	2025	2030	2038	rVB4	26164	46340	2.53%	0.384%
18	15.253	2063	2070	2074	rBV3	15450	22791	1.25%	0.189%
19	15.993	2191	2196	2199	rBV3	16503	26935	1.47%	0.223%
20	16.040	2199	2204	2210	rVB	401738	590833	32.30%	4.901%
21	16.099	2210	2214	2222	rBV	43764	68455	3.74%	0.568%
22	16.240	2230	2238	2252	rVV2	468445	752490	41.14%	6.242%
23	16.469	2272	2277	2284	rBV6	9994	25245	1.38%	0.209%
24	17.491	2445	2451	2462	rBV2	200866	334492	18.29%	2.775%
25	18.061	2542	2548	2554	rBV2	22467	35077	1.92%	0.291%
26	18.361	2593	2599	2608	rBV2	131415	229543	12.55%	1.904%
27	18.432	2608	2611	2620	rVB5	24912	42313	2.31%	0.351%
28	19.336	2759	2765	2769	rBV2	41282	55222	3.02%	0.458%
29	19.530	2792	2798	2802	rBV	17165	26954	1.47%	0.224%
30	19.577	2802	2806	2810	rVB4	25025	31502	1.72%	0.261%
31	19.624	2810	2814	2819	rBV4	22192	35608	1.95%	0.295%
32	19.889	2855	2859	2865	rVB	13273	19296	1.05%	0.160%
33	20.036	2879	2884	2886	rBV3	35553	47781	2.61%	0.396%
34	20.083	2886	2892	2903	rVB	1165859	1572913	85.99%	13.048%
35	20.347	2933	2937	2941	rBV7	12019	20505	1.12%	0.170%
36	20.553	2967	2972	2979	rVB	161100	220759	12.07%	1.831%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121025\
Data File : BG064925.D
Acq On : 10 Dec 2025 17:51
Operator : RC/JU
Sample : Q3814-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-12

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	20.723	2995	3001	3005	rBV	1452503	1829101	100.00%	15.174%
38	20.758	3005	3007	3021	rVB2	280488	440892	24.10%	3.657%
39	21.252	3087	3091	3096	rBV7	15722	26846	1.47%	0.223%
40	21.375	3106	3112	3119	rBV4	64152	136731	7.48%	1.134%
41	21.499	3126	3133	3145	rVB	180242	283316	15.49%	2.350%
42	21.745	3168	3175	3189	rVB2	262445	497007	27.17%	4.123%
43	21.974	3206	3214	3219	rVV	117908	214015	11.70%	1.775%
44	22.016	3219	3221	3228	rVB8	12506	20359	1.11%	0.169%
45	22.468	3291	3298	3304	rBV2	92271	180821	9.89%	1.500%
46	22.538	3304	3310	3326	rVB	165009	367921	20.11%	3.052%
47	24.060	3561	3569	3575	rBV3	33967	78074	4.27%	0.648%
48	24.994	3716	3728	3746	rBV	172631	515205	28.17%	4.274%
49	26.181	3920	3930	3940	rBV3	31776	97778	5.35%	0.811%
50	26.293	3940	3949	3957	rBV7	26605	80019	4.37%	0.664%
51	29.225	4439	4448	4450	rBV8	12053	30537	1.67%	0.253%
52	30.400	4635	4648	4665	rBV8	51523	258482	14.13%	2.144%




Sum of corrected areas: 12054510

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121025\
Data File : BG064925.D
Acq On : 10 Dec 2025 17:51
Operator : RC/JU
Sample : Q3814-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

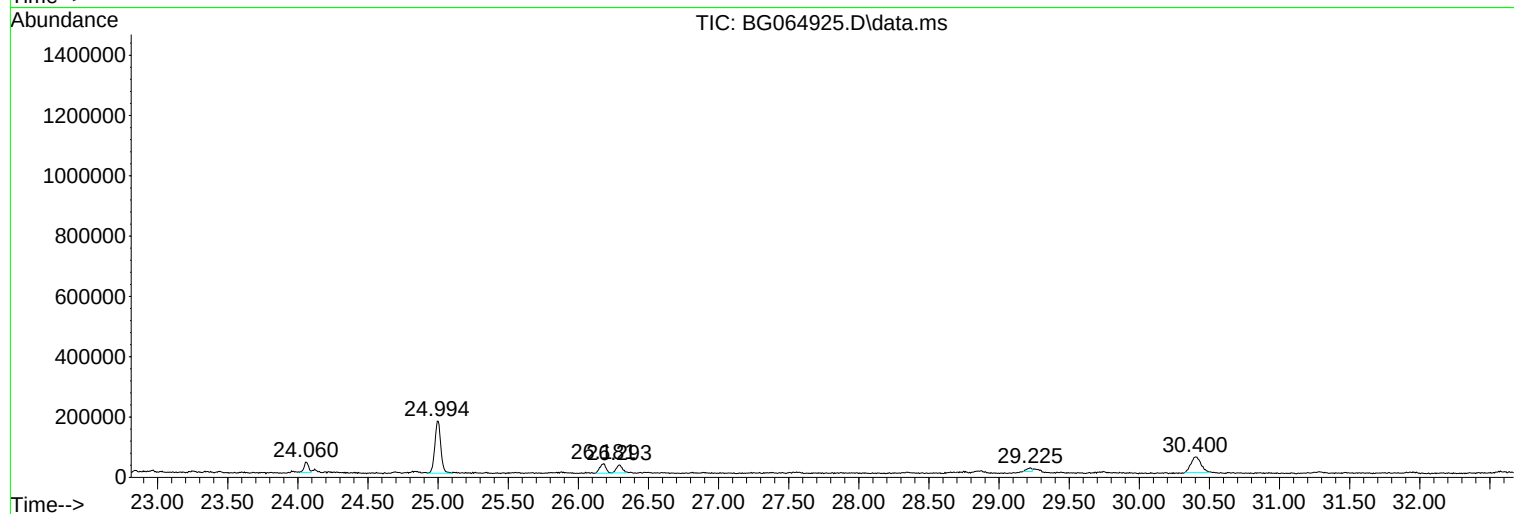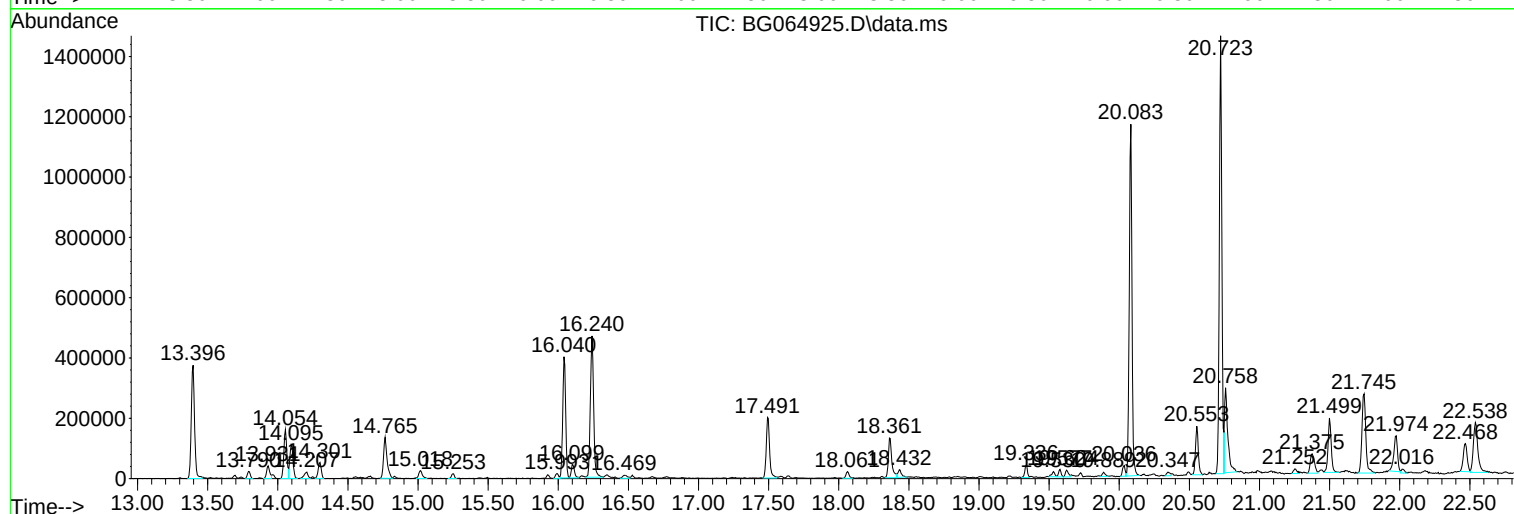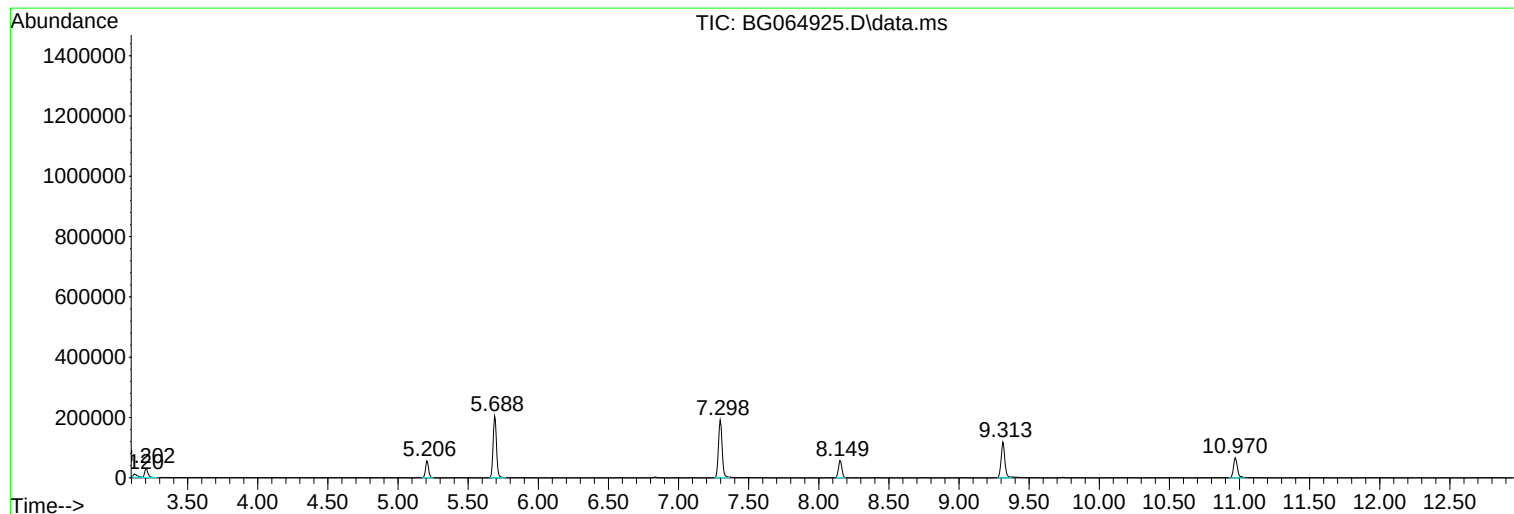

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121025\
Data File : BG064925.D
Acq On : 10 Dec 2025 17:51
Operator : RC/JU
Sample : Q3814-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121025\
Data File : BG064925.D
Acq On : 10 Dec 2025 17:51
Operator : RC/JU
Sample : Q3814-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------