


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121025\
Data File : BG064916.D
Acq On : 10 Dec 2025 10:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 12 17:10:56 2025

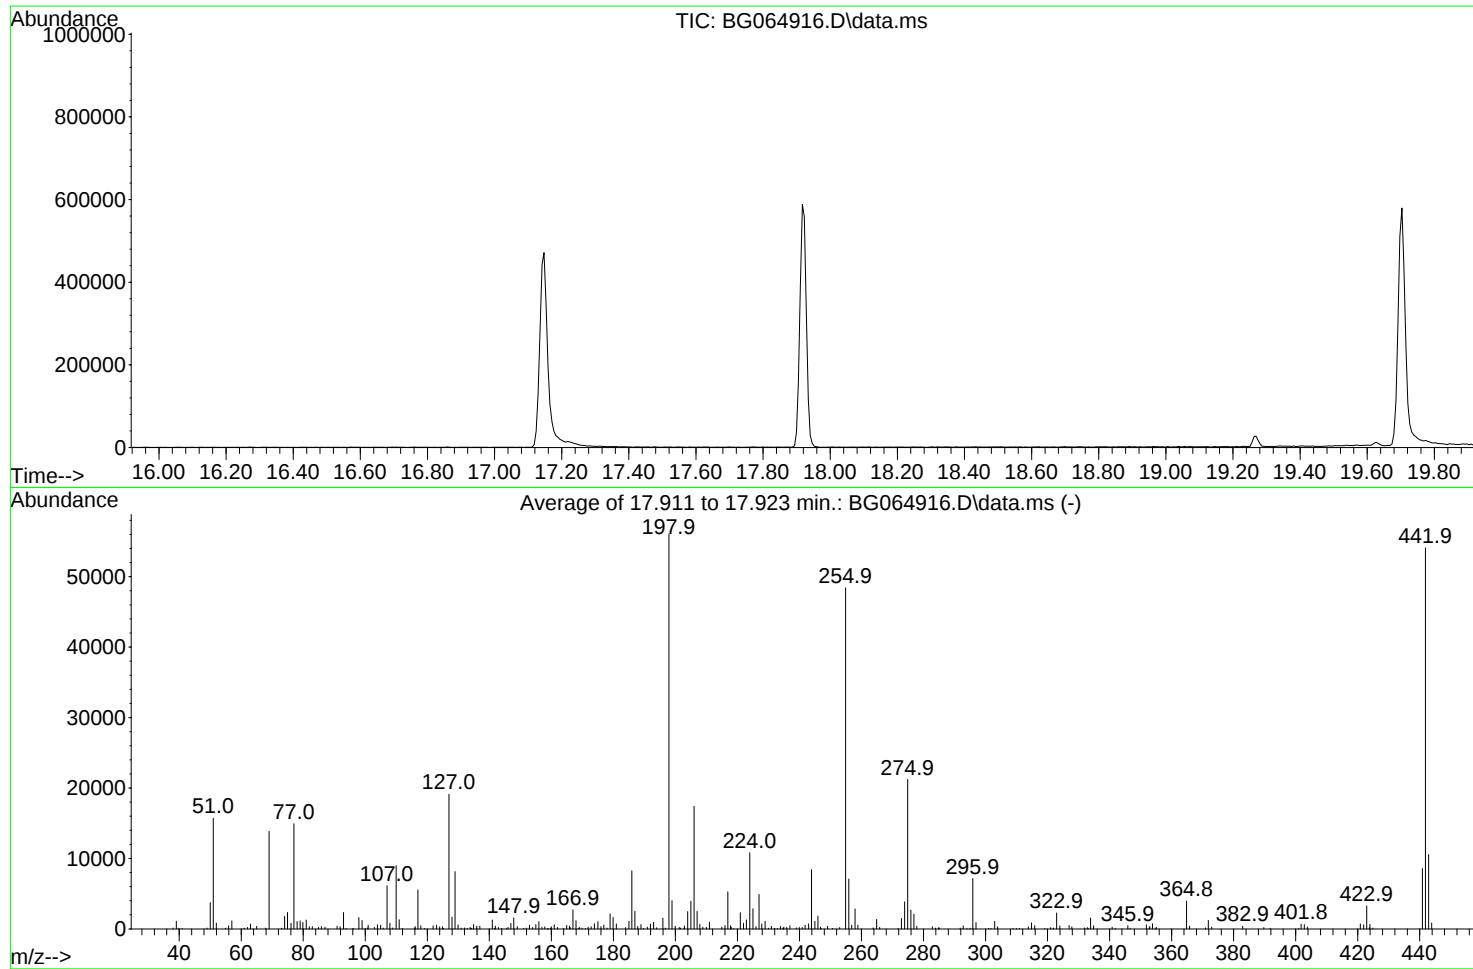




AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.9	131	PASS
69	69	100	100	100.0	13867	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.2	137	PASS
198	198	100	100	100.0	56040	PASS
199	198	5	9	7.2	4010	PASS
365	198	1	100	7.1	3952	PASS
441	443	0.01	150	81.4	8583	PASS
442	442	100	100	100.0	54077	PASS
443	442	15	24	19.5	10550	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121025\
Data File : BG064916.D
Acq On : 10 Dec 2025 10:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 10 11:23:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

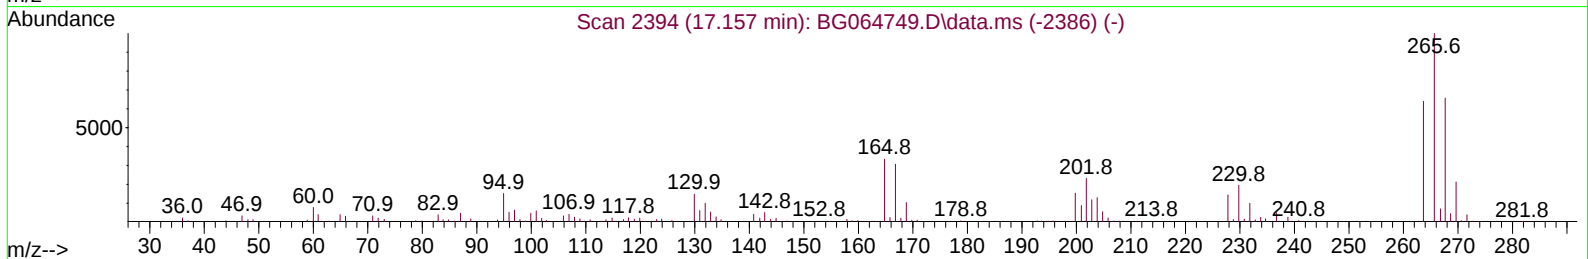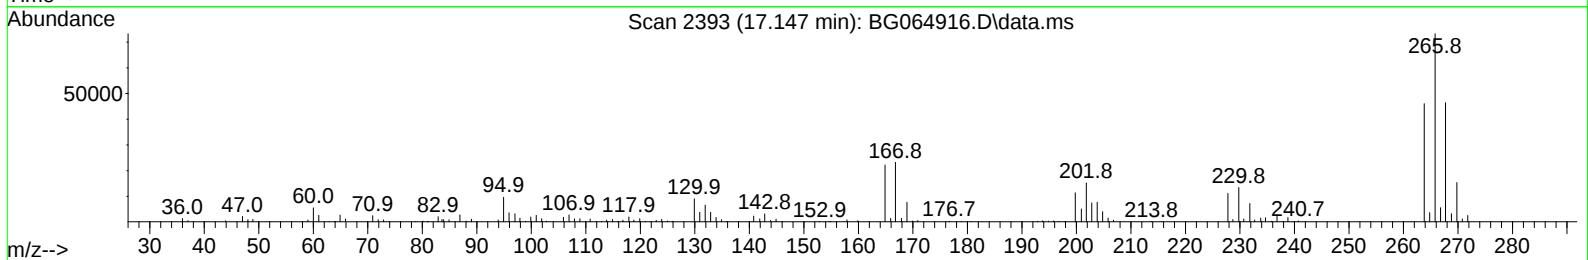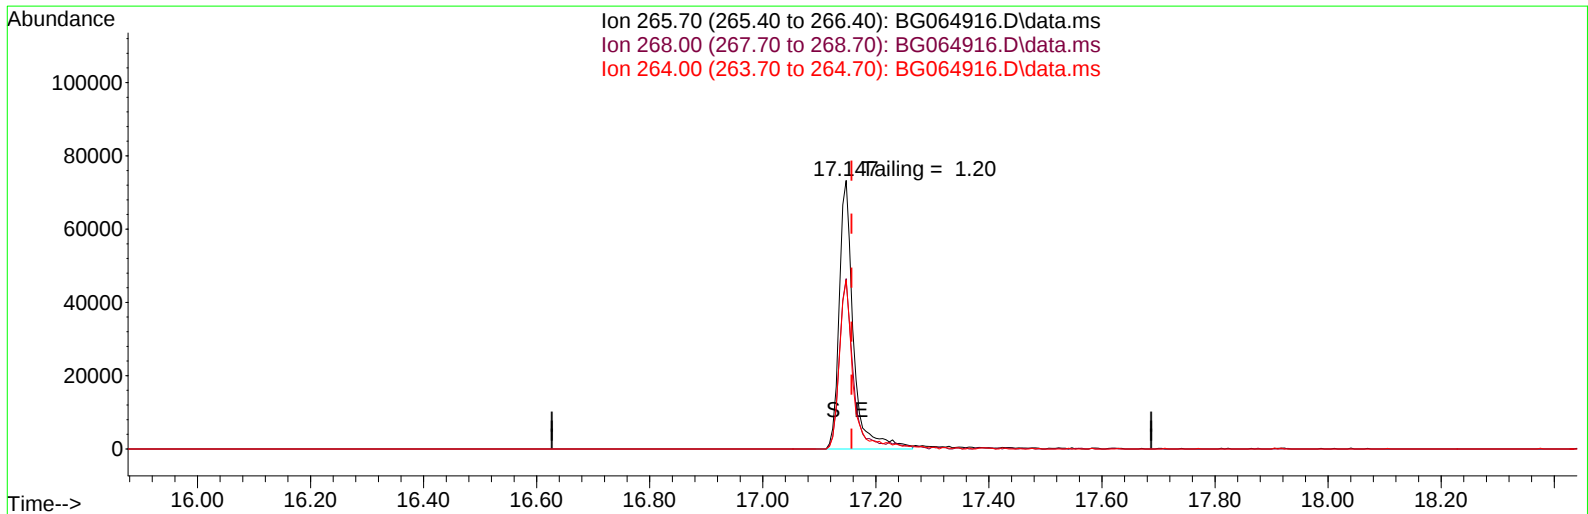

TIC: BG064916.D\data.ms

(70) Pentachlorophenol (C)

17.147min (-0.010) 29506.23 ng




response 128464

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.10	63.40
264.00	64.00	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121025\
Data File : BG064916.D
Acq On : 10 Dec 2025 10:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 10 11:23:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

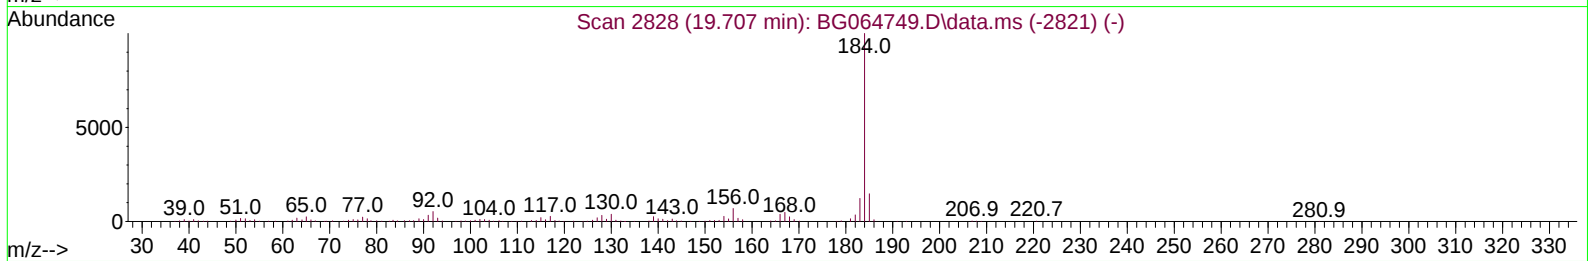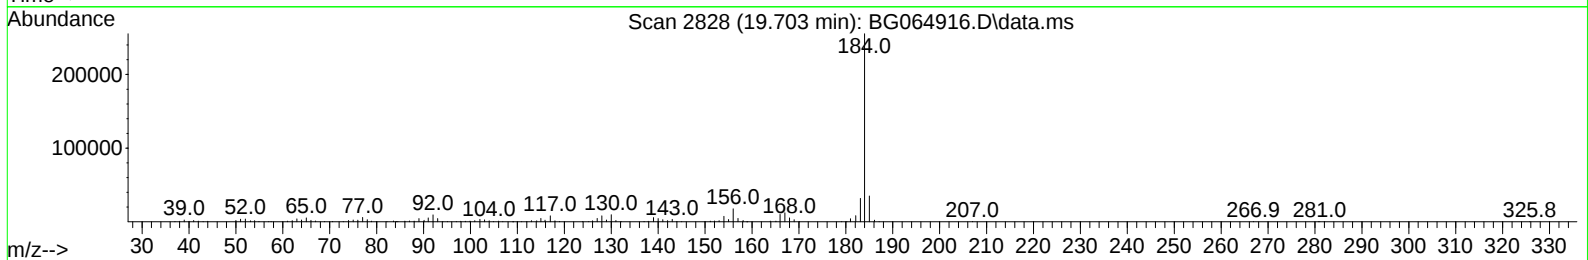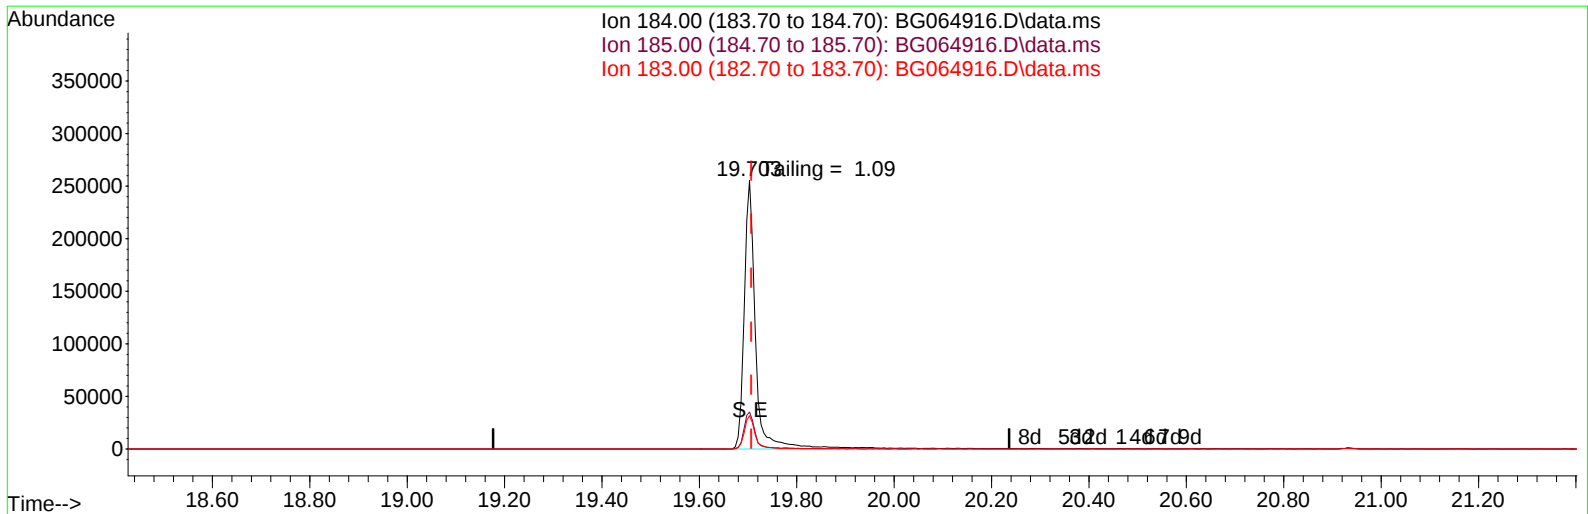

TIC: BG064916.D\data.ms

(77) Benzidine

19.703min (-0.004) 218453.11 ng m

response 425251

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.76
183.00	12.20	12.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/10/2025	BNA_G	<u>BG064916.D</u>
Compound Name	Response	Retention Time
DDT	287569	20.931
DDD	4919	20.496
DDE	542	19.991
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5461	293030	1.86

Instrument :
BNA_G
ClientSampleId :
DFTPP