
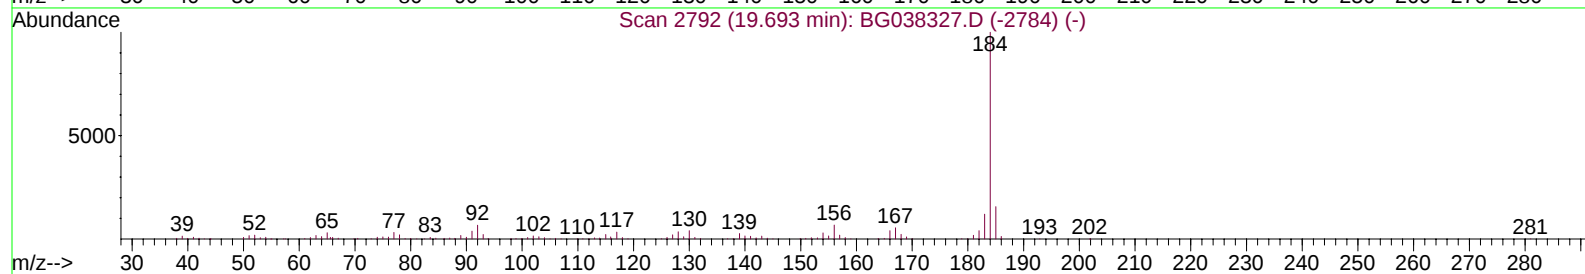
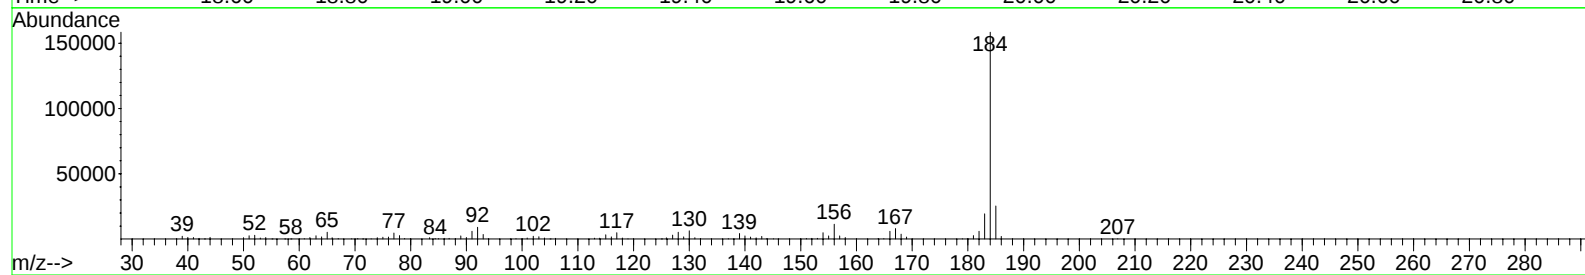


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121118\
Data File : BG038471.D
Acq On : 11 Dec 2018 15:22
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 16:33:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 17:15:40 2018
Response via : Initial Calibration

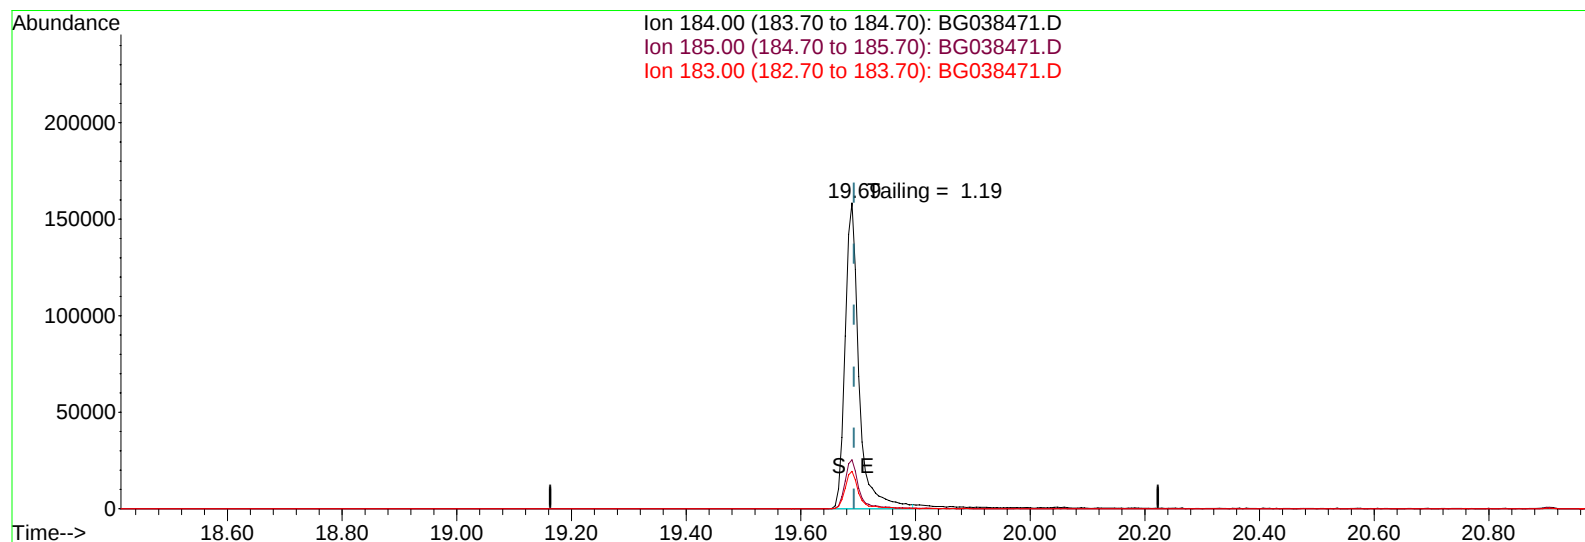

TIC: BG038471.D

(77) Benzidine




19.689min (-0.003) 41370.72ng

response 272228

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.00
183.00	12.70	12.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121118\
Data File : BG038471.D
Acq On : 11 Dec 2018 15:22
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 16:33:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 17:15:40 2018
Response via : Initial Calibration

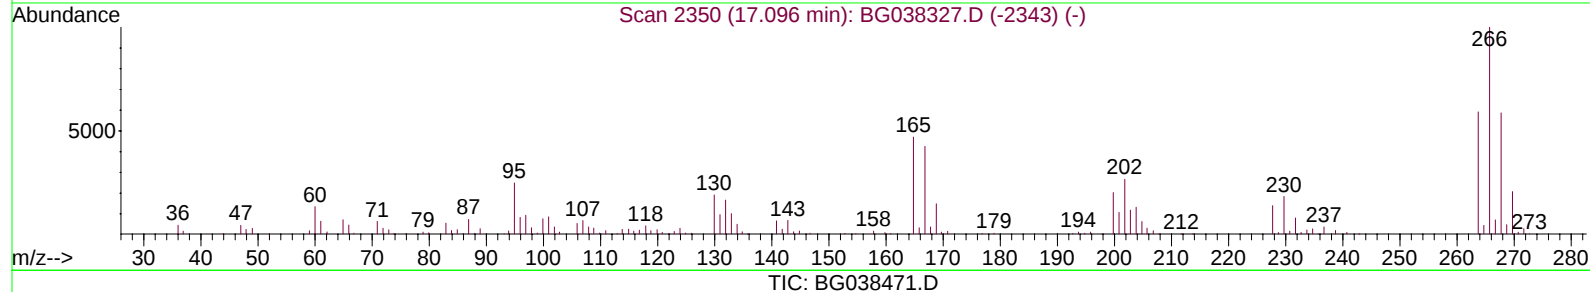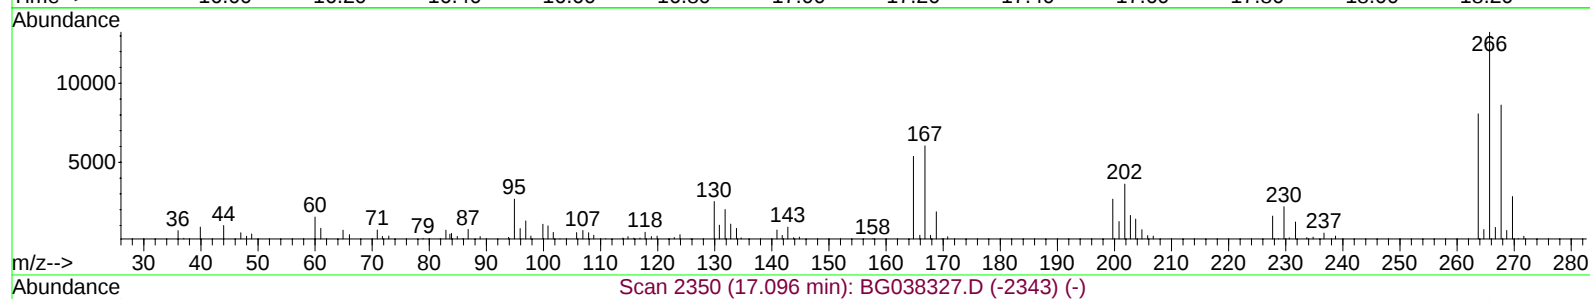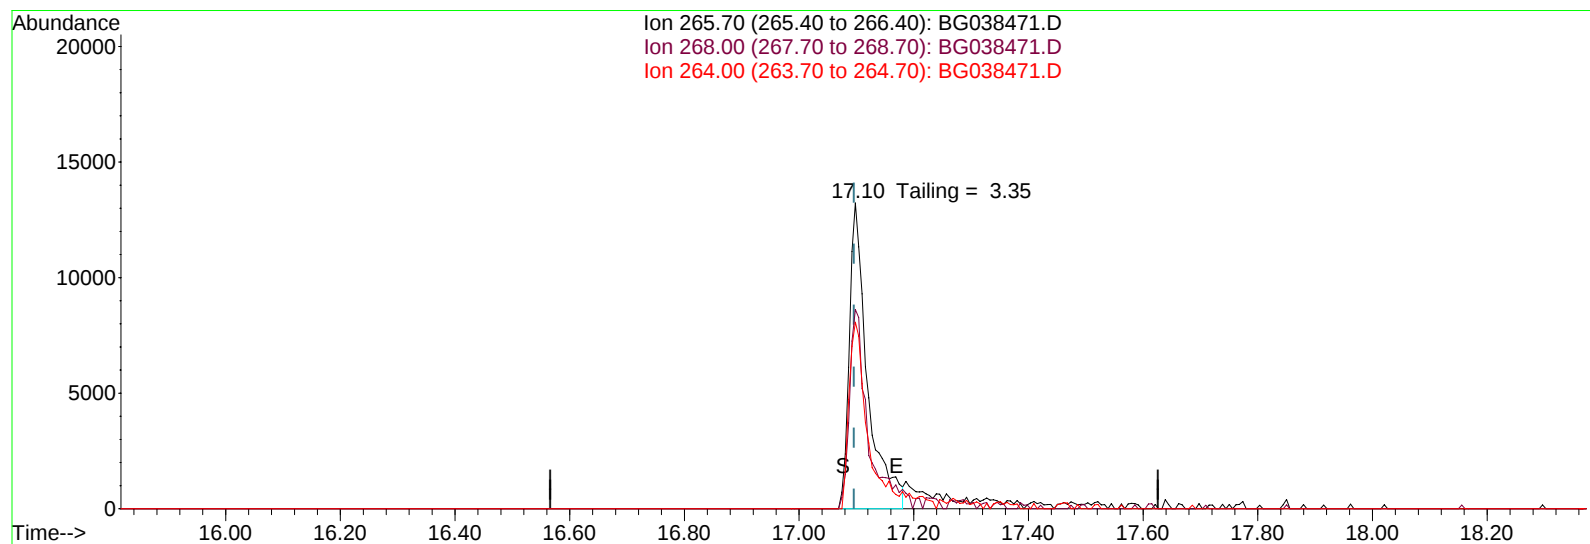

(70) Pentachlorophenol (C)

17.098min (+0.002) 12391.70ng

response 29402

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	70.36
264.00	73.60	66.68
0.00	0.00	0.00