


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121118\
 Data File : BG038471.D
 Acq On : 11 Dec 2018 15:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 04 17:15:40 2018

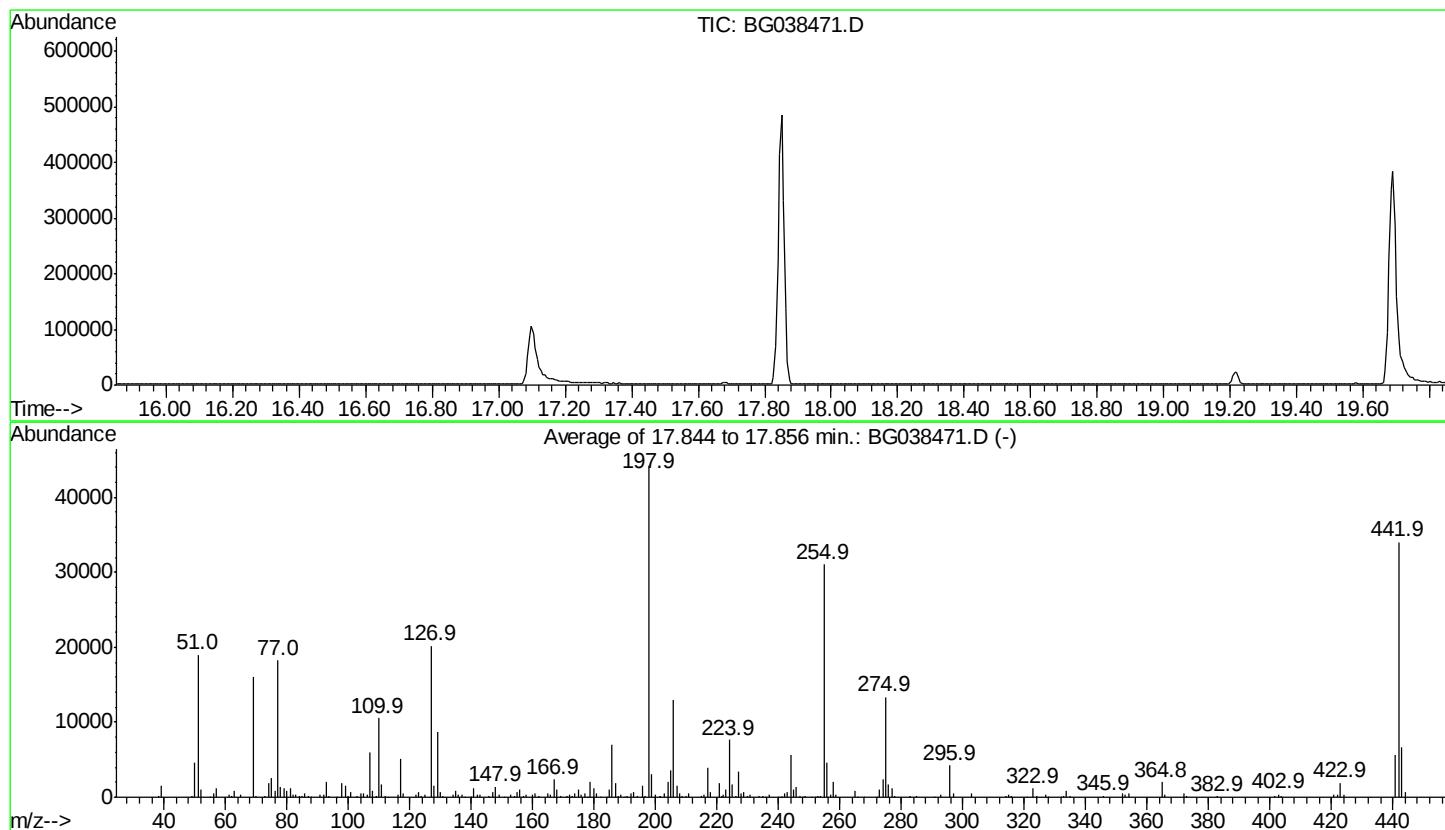

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.0	19018	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.3	16049	PASS
70	69	0.00	2	0.8	132	PASS
127	198	10	80	45.7	20221	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	44216	PASS
199	198	5	9	6.9	3063	PASS
275	198	10	60	30.2	13371	PASS
365	198	1	100	4.6	2014	PASS
441	198	0.01	100	12.8	5674	PASS
442	198	50	100	77.0	34032	PASS
443	442	15	24	19.7	6709	PASS