


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121118\
 Data File : BG038488.D
 Acq On : 12 Dec 2018 4:30
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 04 17:15:40 2018

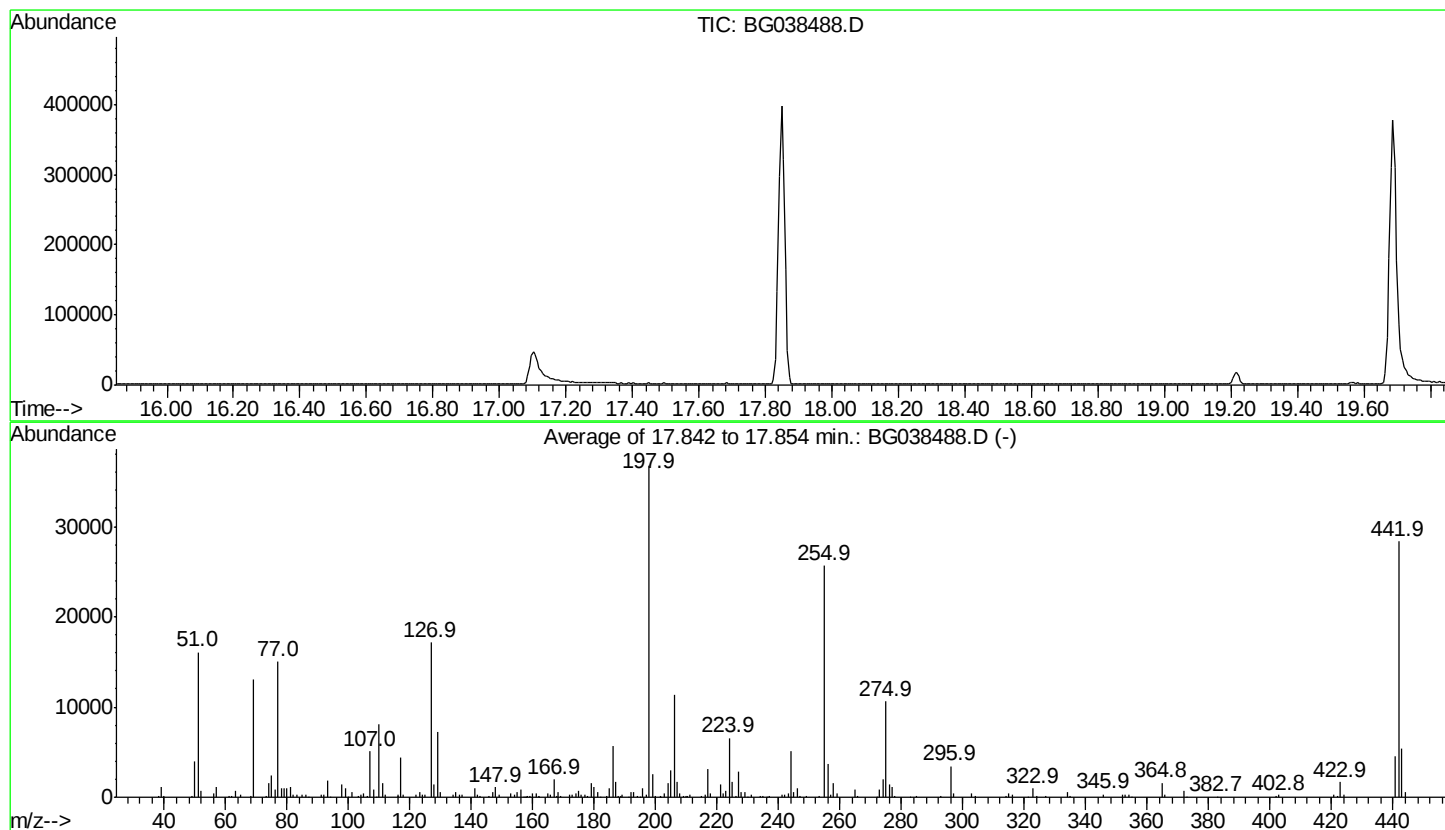

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.7	16047	PASS
68	69	0.00	2	1.2	163	PASS
69	198	0.00	100	35.7	13120	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.6	17110	PASS
197	198	0.00	2	0.9	327	PASS
198	198	100	100	100.0	36754	PASS
199	198	5	9	6.8	2503	PASS
275	198	10	60	28.9	10626	PASS
365	198	1	100	4.3	1598	PASS
441	198	0.01	100	12.5	4604	PASS
442	198	50	100	77.2	28365	PASS
443	442	15	24	18.8	5326	PASS