
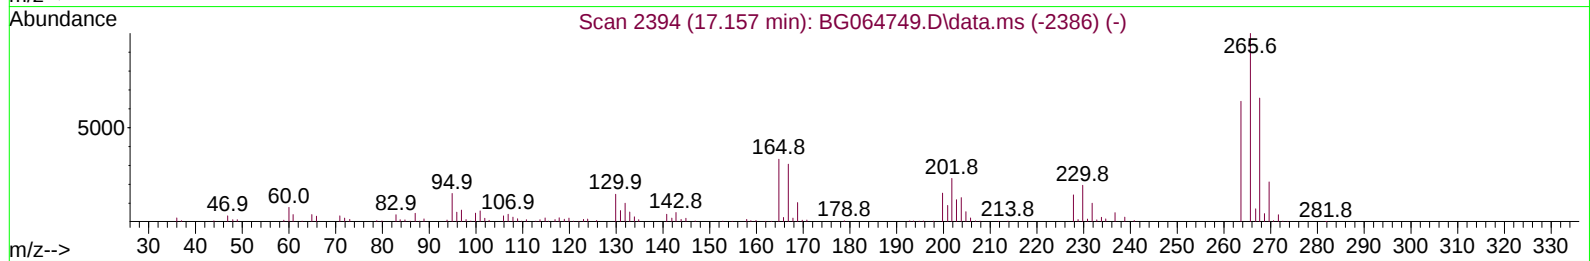
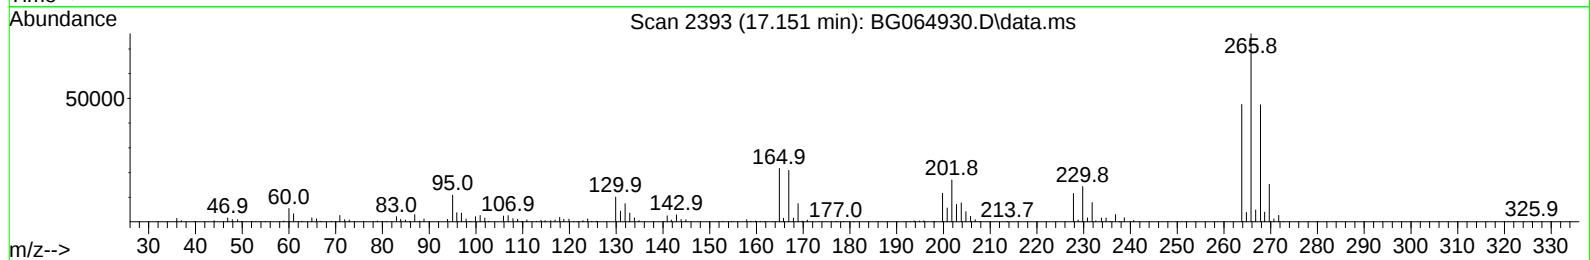


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121125\
Data File : BG064930.D
Acq On : 11 Dec 2025 11:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 12:26:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

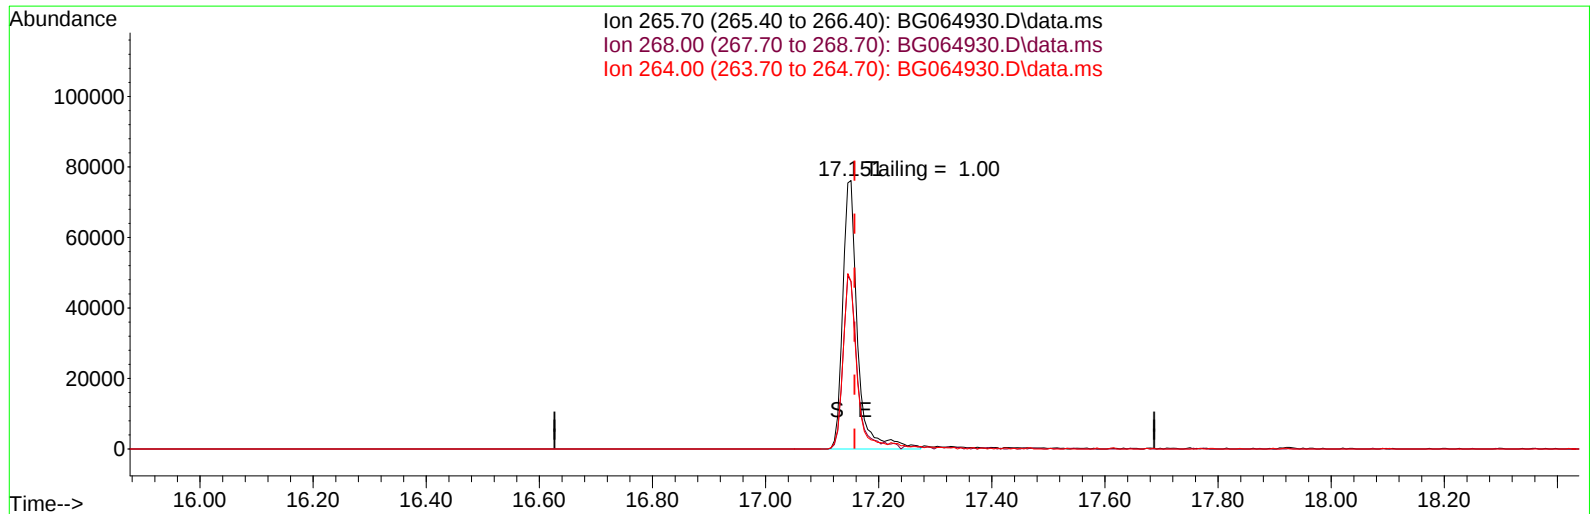

TIC: BG064930.D\data.ms

(70) Pentachlorophenol (C)




17.151min (-0.006) 25329.71 ng

response 132745

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.10	67.52
264.00	64.00	62.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121125\
Data File : BG064930.D
Acq On : 11 Dec 2025 11:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 12:26:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

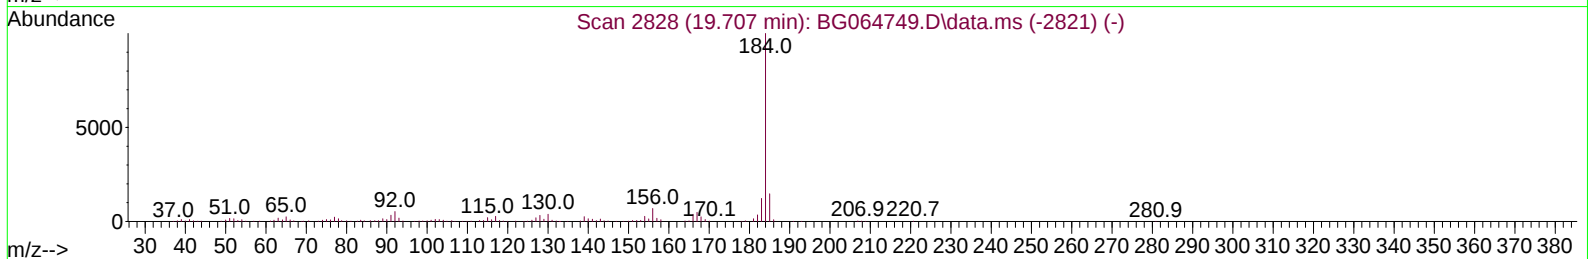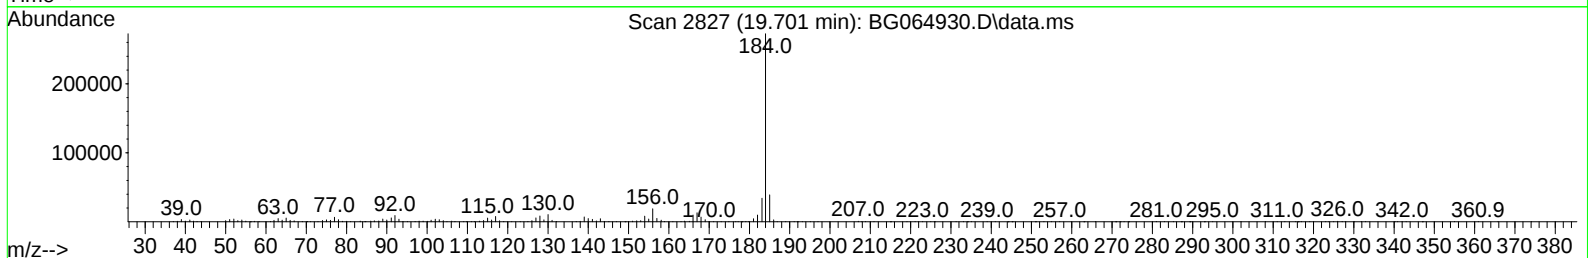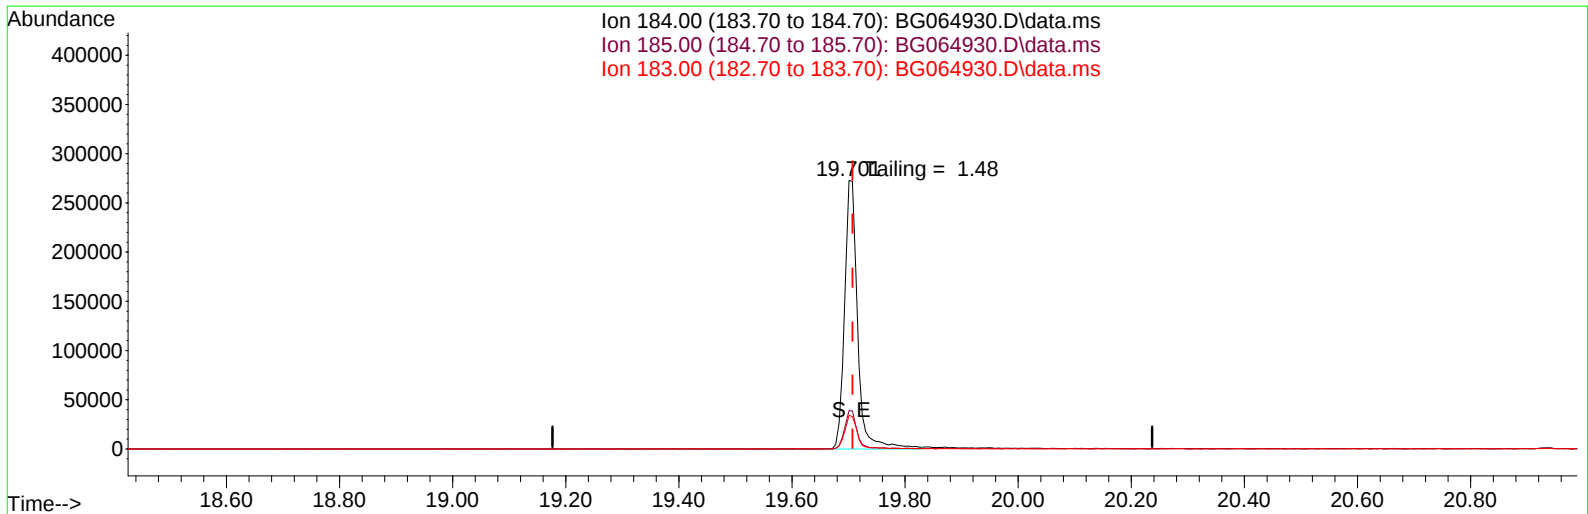

TIC: BG064930.D\data.ms

(77) Benzidine

19.701min (-0.006) 52176.87 ng

response 437532

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.28
183.00	12.20	12.50
0.00	0.00	0.00