

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121125\
 Data File : BG064932.D
 Acq On : 11 Dec 2025 13:16
 Operator : RC/JU
 Sample : PB170902BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB170902BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG064932.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.202	353	360	368	rBB	75529	117293	4.10%	1.404%
2	5.690	436	443	451	rBV	303930	489684	17.12%	5.860%
3	7.300	709	717	731	rBV	287000	510017	17.84%	6.103%
4	8.152	856	862	871	rBV	56603	93179	3.26%	1.115%
5	9.315	1052	1060	1071	rBV	166350	321625	11.25%	3.849%
6	10.972	1333	1342	1348	rBV	62165	119211	4.17%	1.426%
7	13.398	1748	1755	1772	rBV	587100	979475	34.25%	11.720%
8	14.767	1980	1988	2004	rBB	134586	230101	8.05%	2.753%
9	16.242	2232	2239	2258	rBV3	721368	1222759	42.76%	14.632%
10	17.499	2446	2453	2463	rBV2	227755	373655	13.07%	4.471%
11	20.085	2887	2893	2905	rBV	2121820	2859592	100.00%	34.218%
12	21.747	3169	3176	3187	rBV2	287108	538473	18.83%	6.443%
13	25.008	3723	3731	3743	rVB	171113	501915	17.55%	6.006%




Sum of corrected areas: 8356979

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121125\
Data File : BG064932.D
Acq On : 11 Dec 2025 13:16
Operator : RC/JU
Sample : PB170902BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB170902BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

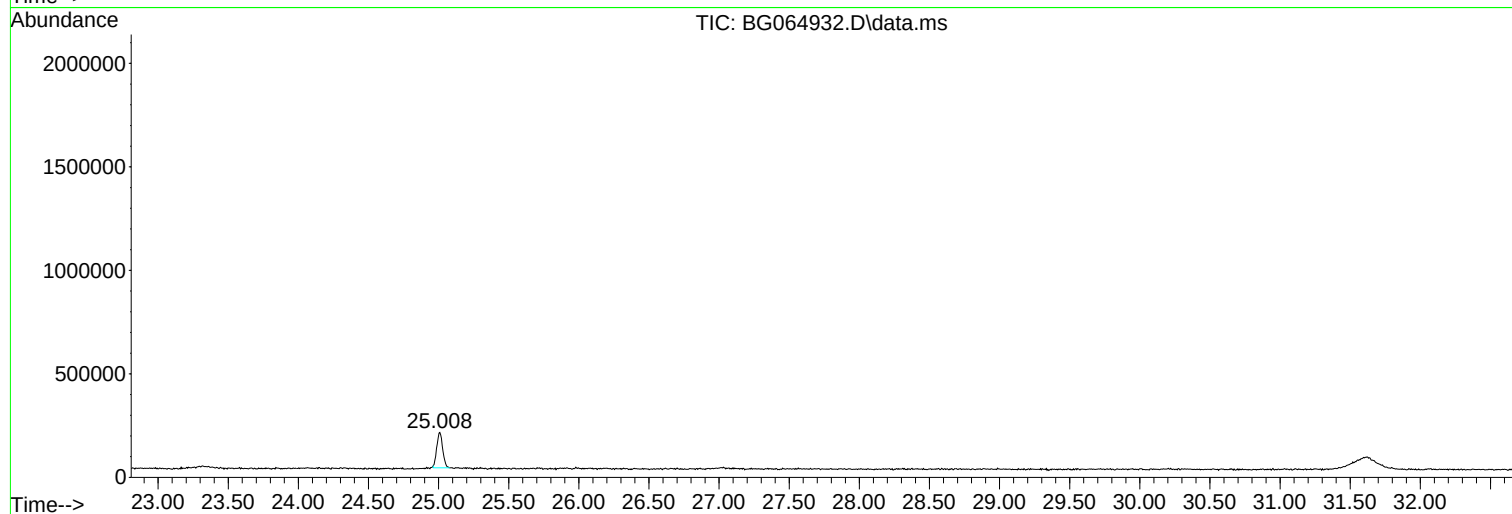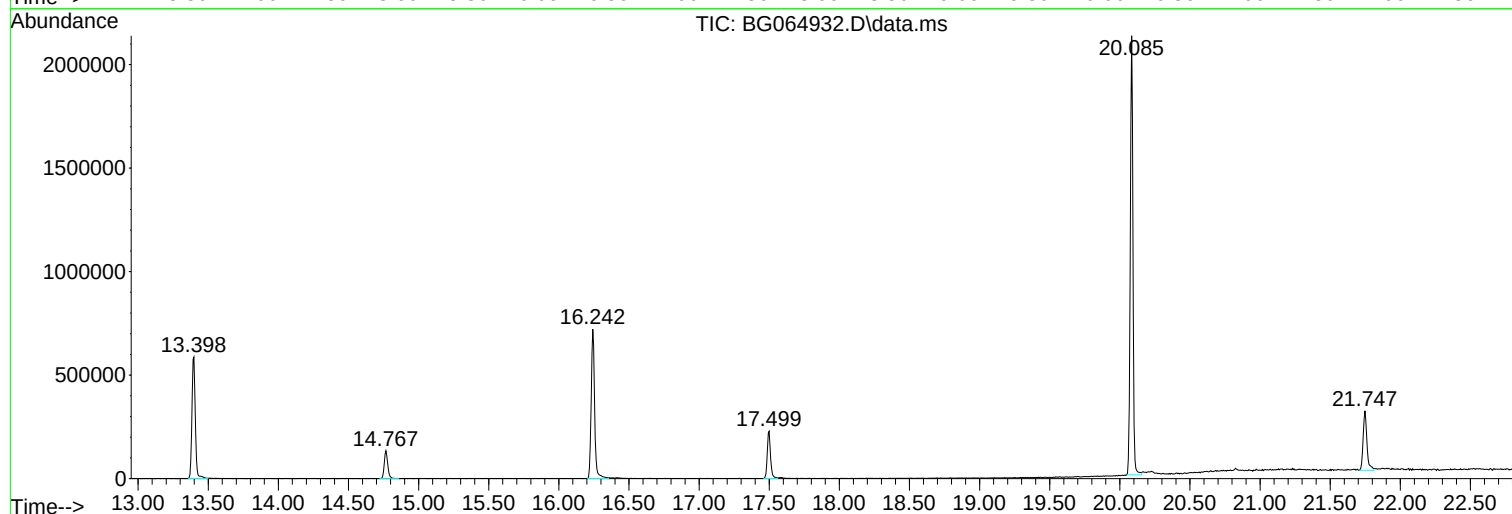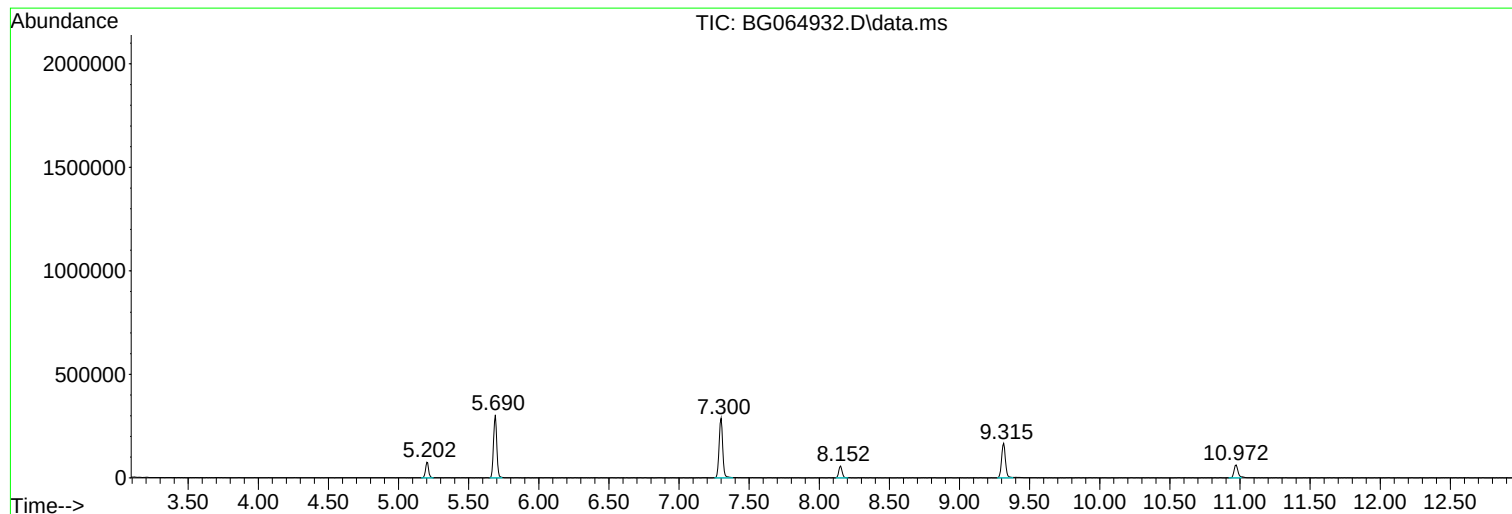

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121125\
Data File : BG064932.D
Acq On : 11 Dec 2025 13:16
Operator : RC/JU
Sample : PB170902BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB170902BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121125\
Data File : BG064932.D
Acq On : 11 Dec 2025 13:16
Operator : RC/JU
Sample : PB170902BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB170902BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------