


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112125\
Data File : BG064930.D
Acq On : 11 Dec 2025 11:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 12 17:10:56 2025

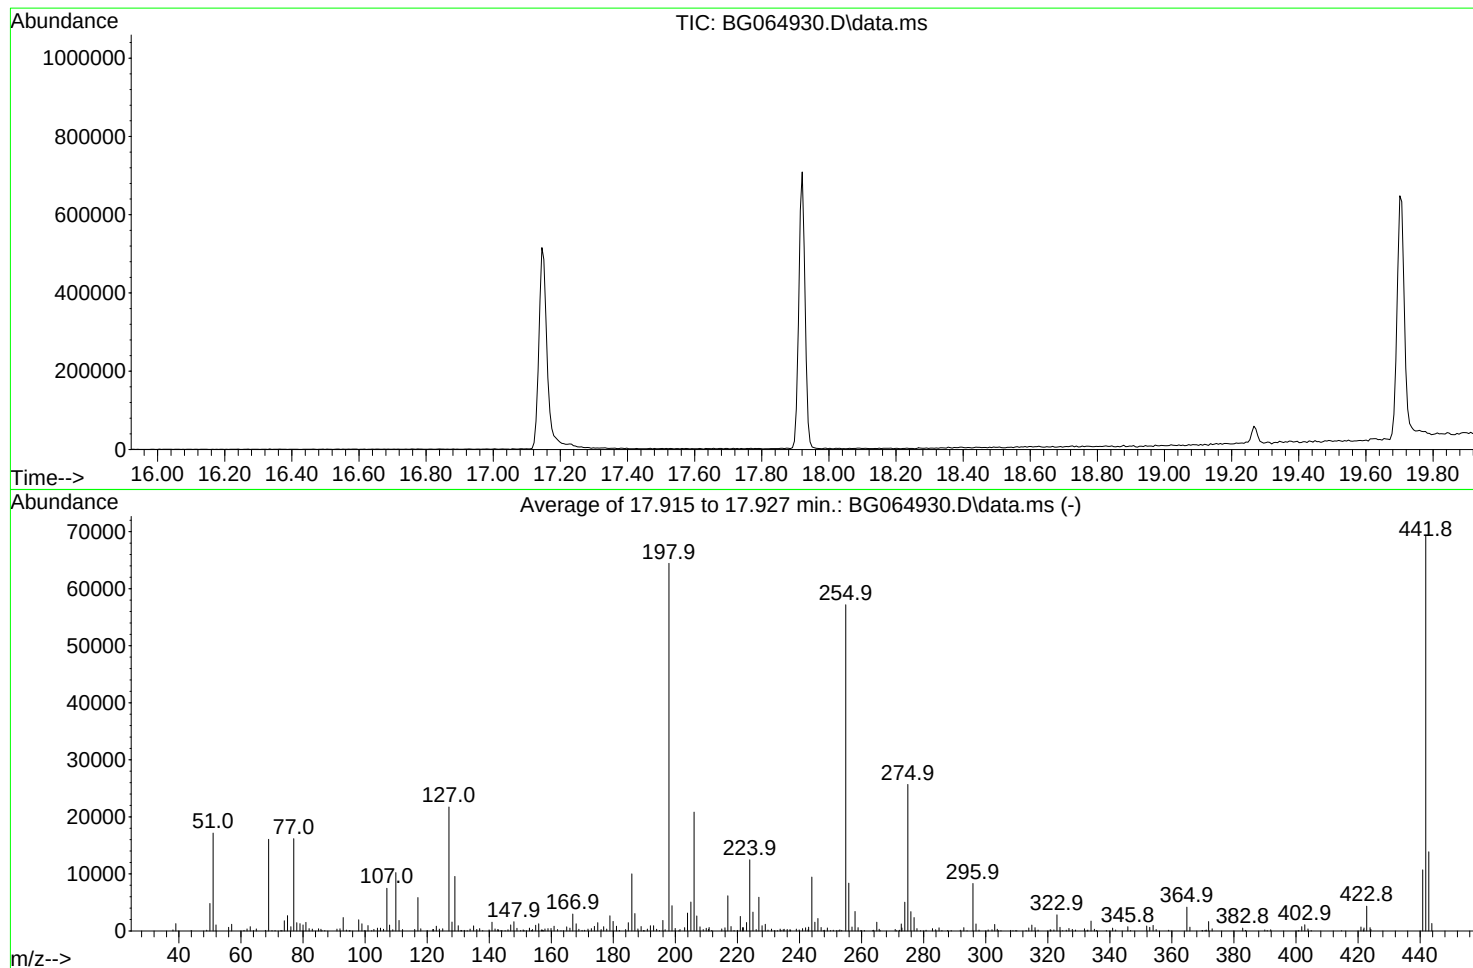




AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.7	108	PASS
69	69	100	100	100.0	16057	PASS
70	69	0.00	2	0.4	60	PASS
197	198	0.00	2	0.3	223	PASS
198	198	100	100	100.0	64448	PASS
199	198	5	9	6.9	4435	PASS
365	198	1	100	6.5	4159	PASS
441	443	0.01	150	77.1	10692	PASS
442	442	100	100	100.0	69224	PASS
443	442	15	24	20.0	13869	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121125\
Data File : BG064930.D
Acq On : 11 Dec 2025 11:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 11 12:26:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

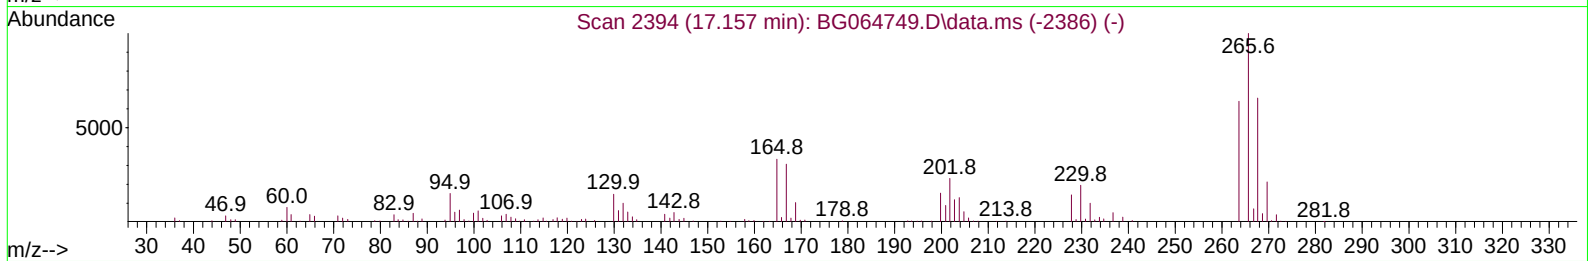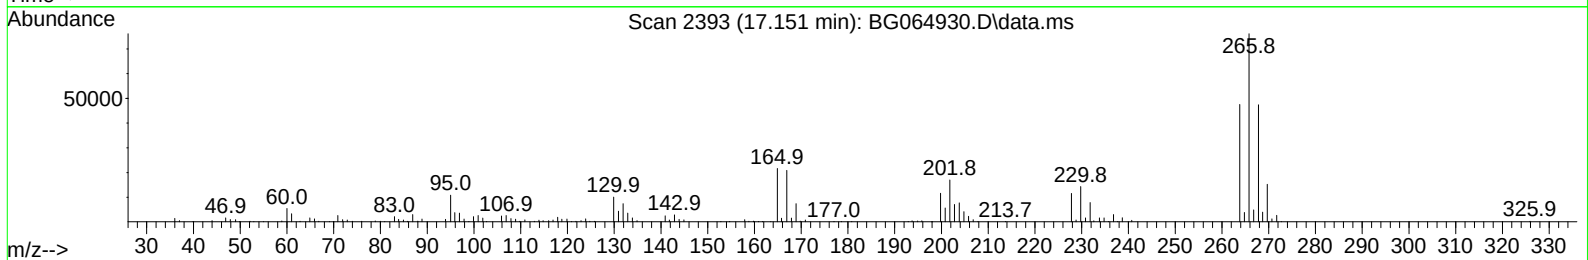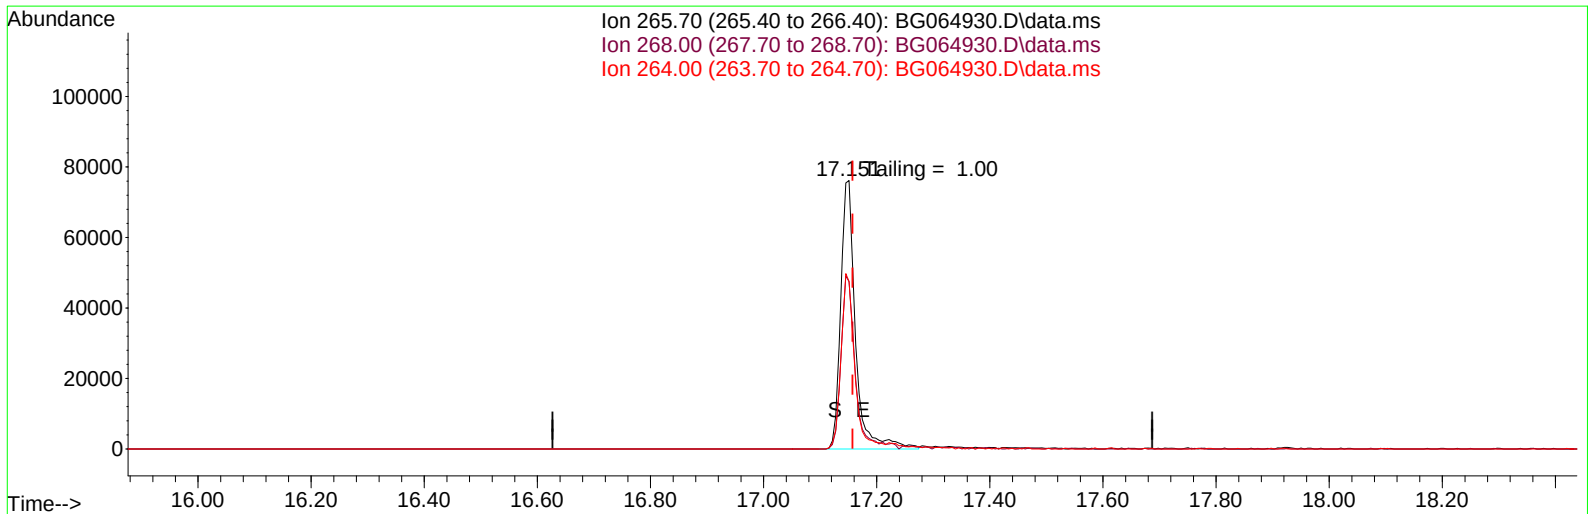

TIC: BG064930.D\data.ms

(70) Pentachlorophenol (C)

17.151min (-0.006) 25329.71 ng




response 132745

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.10	67.52
264.00	64.00	62.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121125\
Data File : BG064930.D
Acq On : 11 Dec 2025 11:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 11 12:26:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

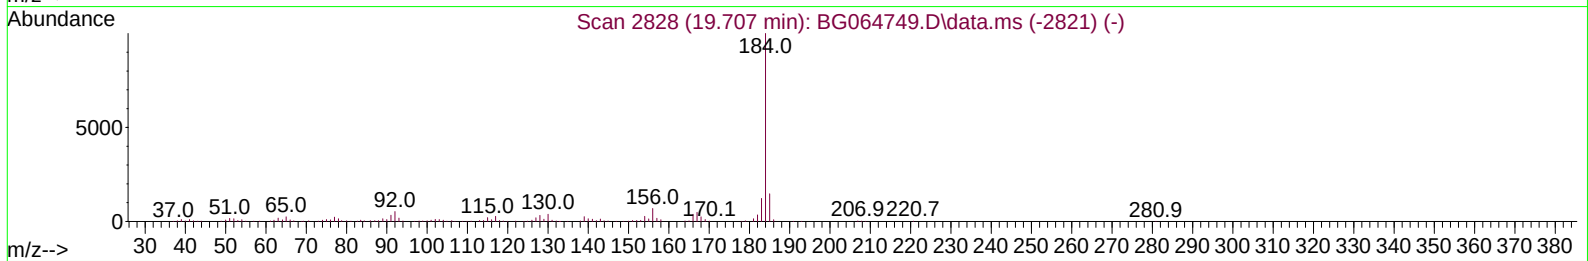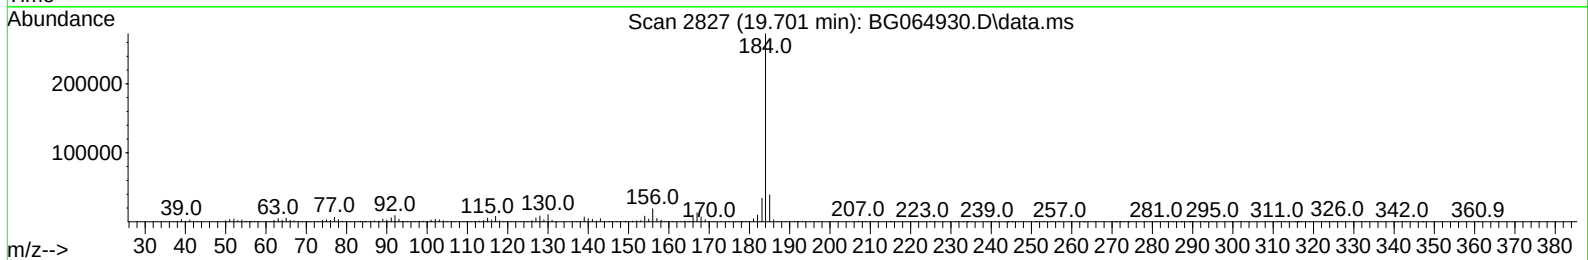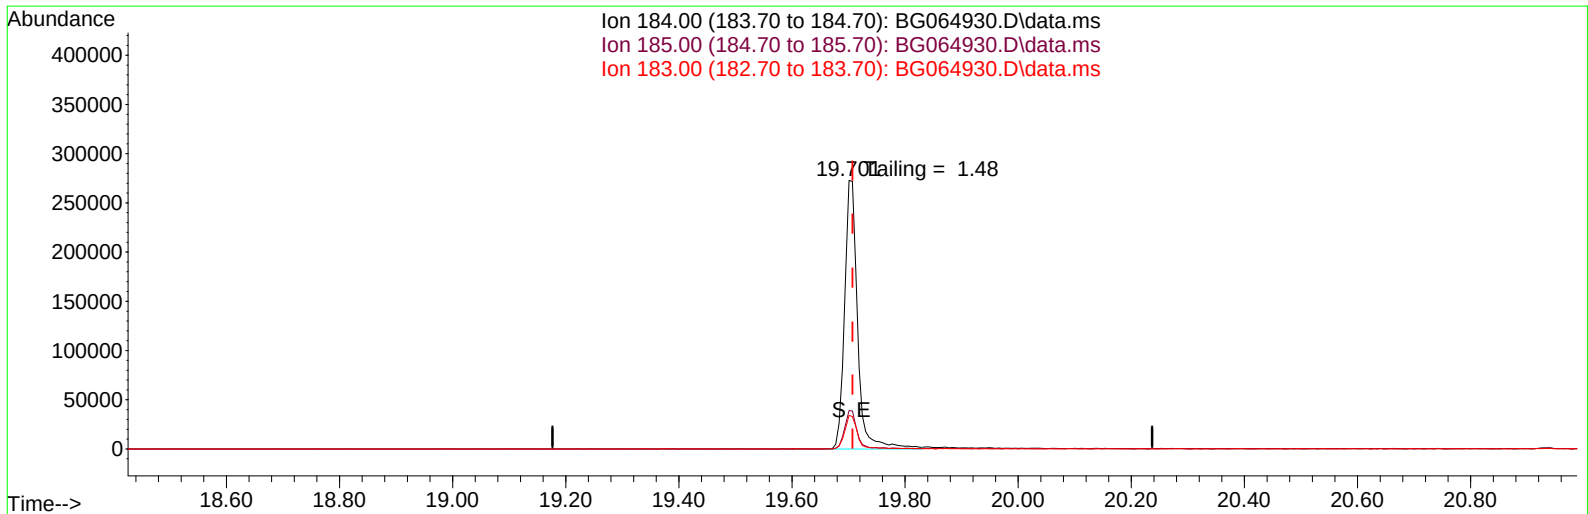

TIC: BG064930.D\data.ms

(77) Benzidine

19.701min (-0.006) 52176.87 ng

response 437532

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.28
183.00	12.20	12.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/11/2025	BNA_G	<u>BG064930.D</u>
Compound Name	Response	Retention Time
DDT	287917	20.935
DDD	7755	20.494
DDE	143	19.971
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7898	295815	2.67

Instrument :
BNA_G
ClientSampleId :
DFTPP