


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121218\
Data File : BG038494.D
Acq On : 12 Dec 2018 9:03
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 12 15:26:27 2018

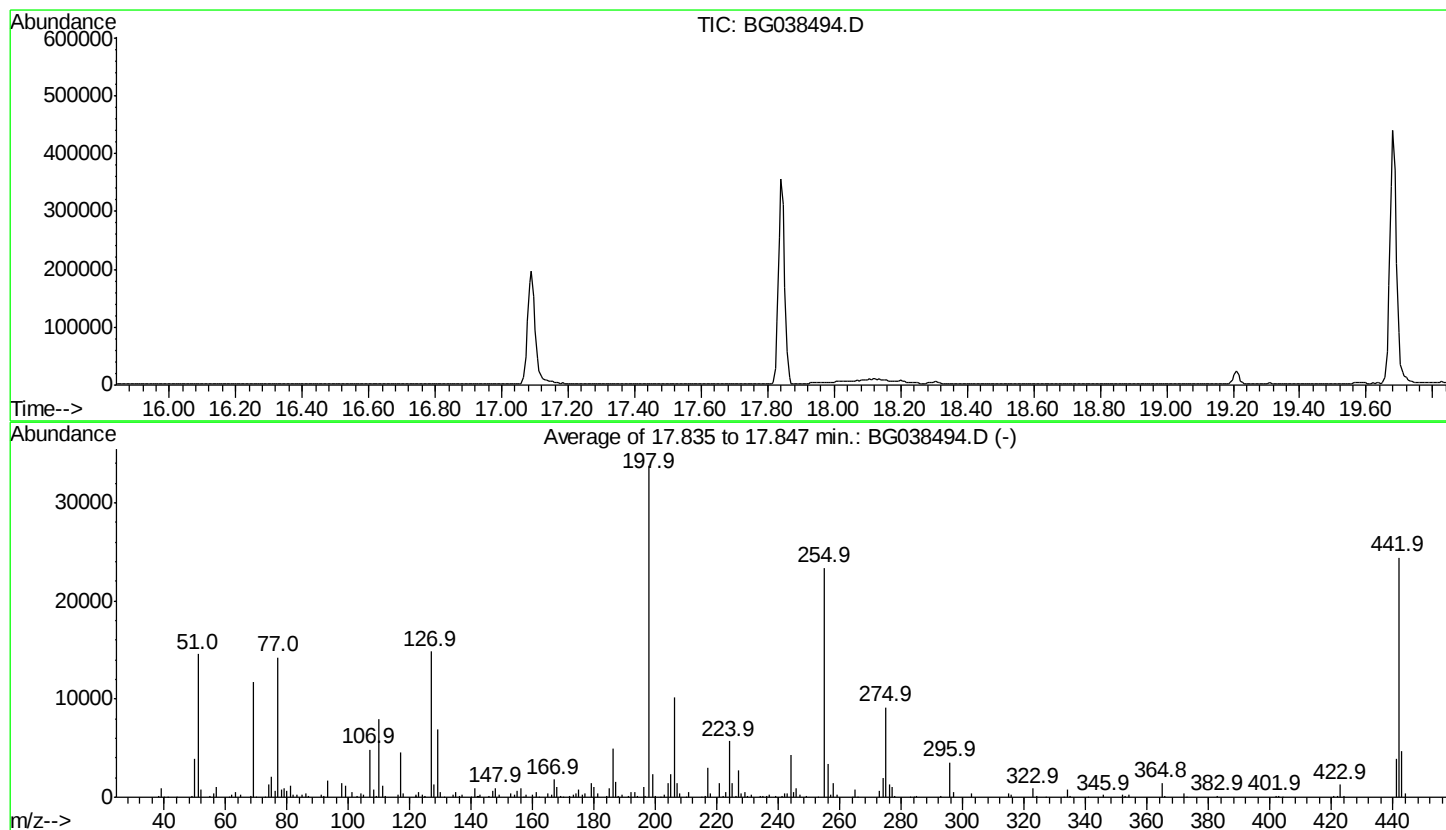

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	14584	PASS
68	69	0.00	2	1.7	196	PASS
69	198	0.00	100	34.8	11761	PASS
70	69	0.00	2	0.4	52	PASS
127	198	10	80	44.0	14860	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	33800	PASS
199	198	5	9	7.0	2371	PASS
275	198	10	60	27.1	9143	PASS
365	198	1	100	4.3	1470	PASS
441	198	0.01	100	11.5	3889	PASS
442	198	50	100	72.3	24427	PASS
443	442	15	24	19.0	4644	PASS