


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121218\
 Data File : BG038521.D
 Acq On : 13 Dec 2018 7:34
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

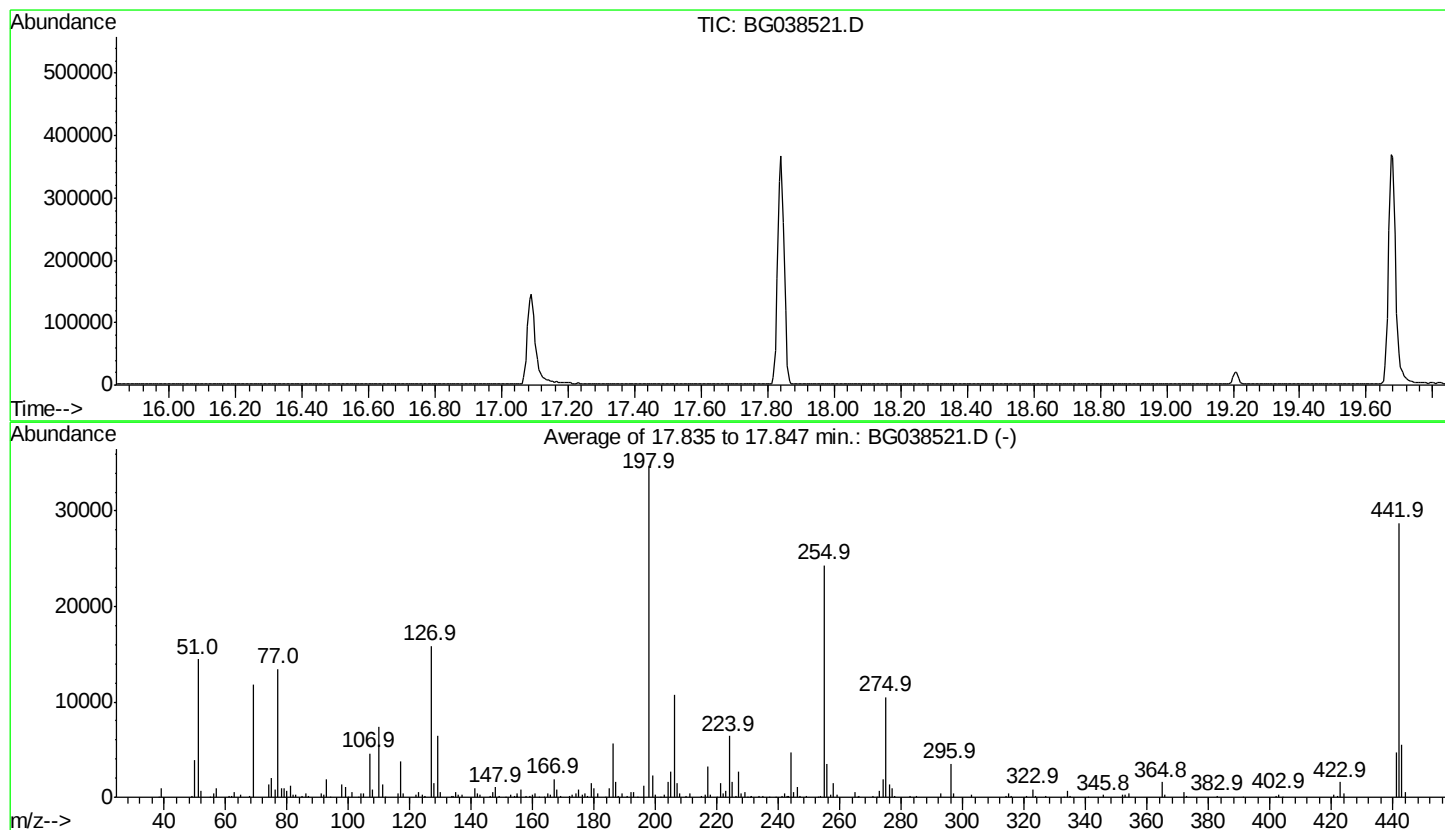

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.6	14466	PASS
68	69	0.00	2	1.2	144	PASS
69	198	0.00	100	33.8	11754	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.6	15836	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	34765	PASS
199	198	5	9	6.4	2242	PASS
275	198	10	60	30.3	10521	PASS
365	198	1	100	4.6	1610	PASS
441	198	0.01	100	13.4	4651	PASS
442	198	50	100	82.7	28736	PASS
443	442	15	24	19.0	5470	PASS