
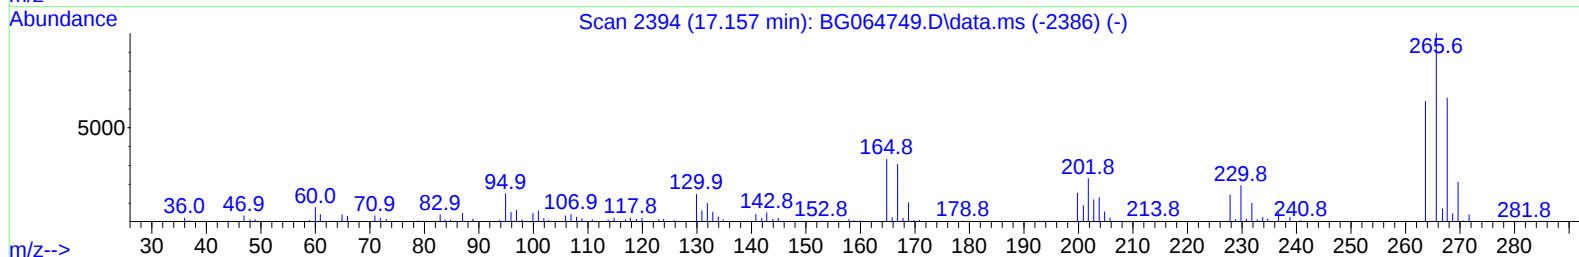
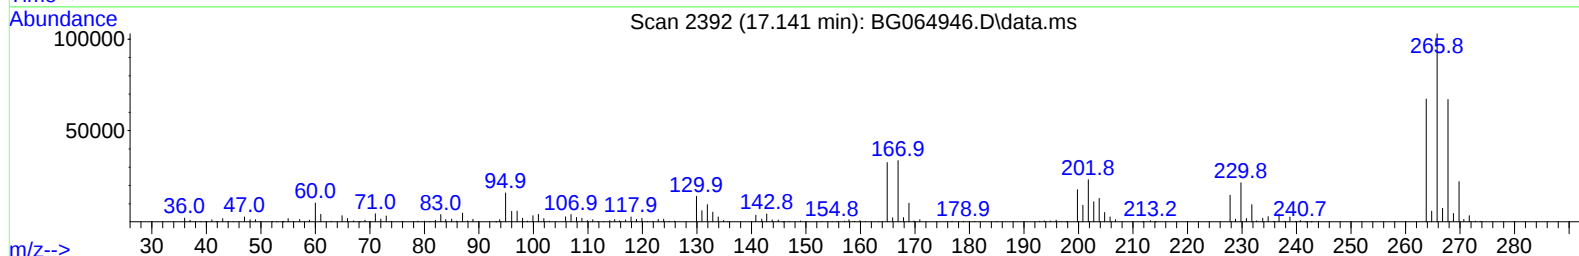


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121225\
Data File : BG064946.D
Acq On : 12 Dec 2025 10:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 11:58:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

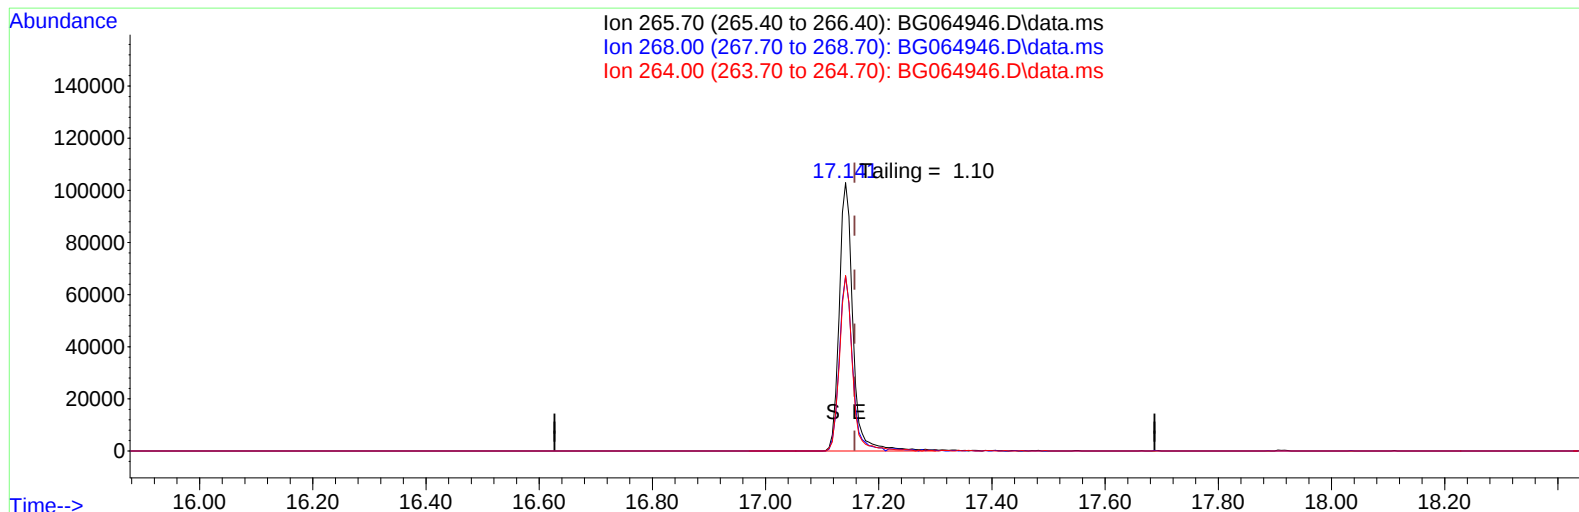

TIC: BG064946.D\data.ms

(70) Pentachlorophenol (C)




17.141min (-0.016) 312436.63 ng

response 172059

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.10	65.12
264.00	64.00	65.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121225\
Data File : BG064946.D
Acq On : 12 Dec 2025 10:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 11:58:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 17:10:56 2025
Response via : Initial Calibration

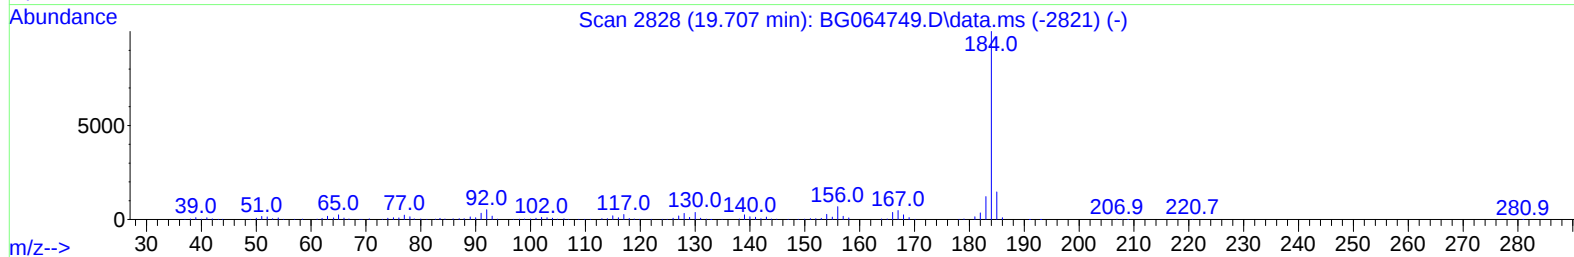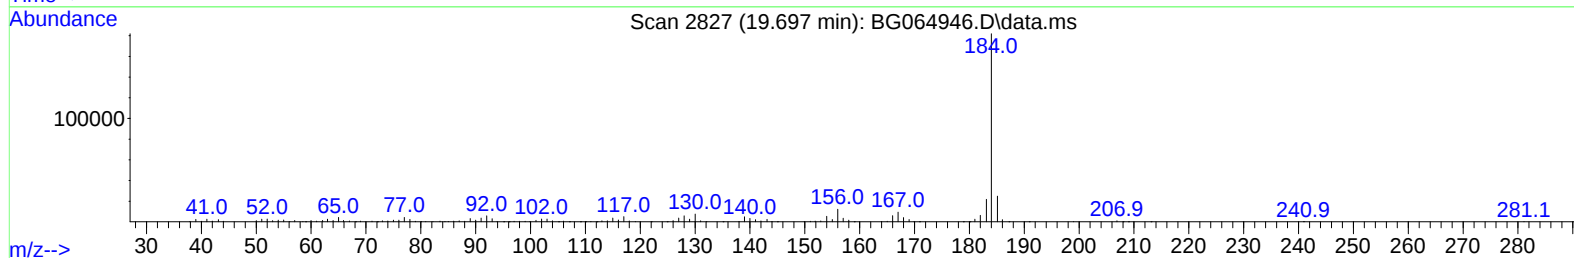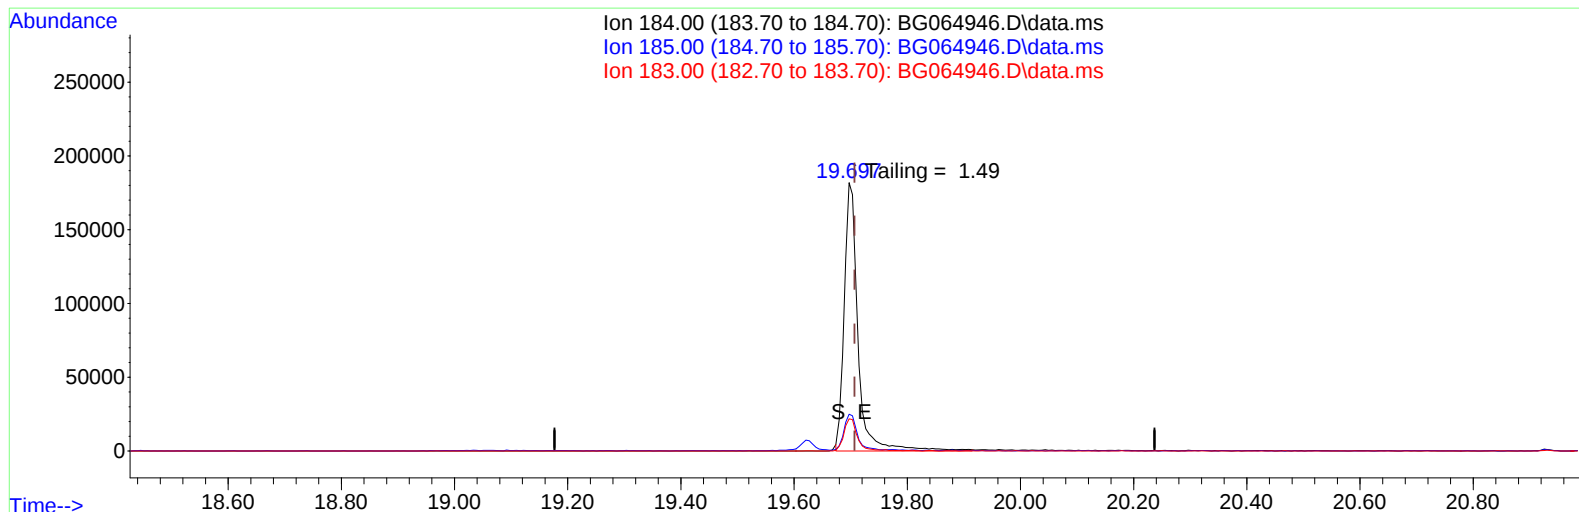

TIC: BG064946.D\data.ms

(77) Benzidine

19.697min (-0.009) 183504.27 ng

response 307757

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.72
183.00	12.20	12.02
0.00	0.00	0.00