
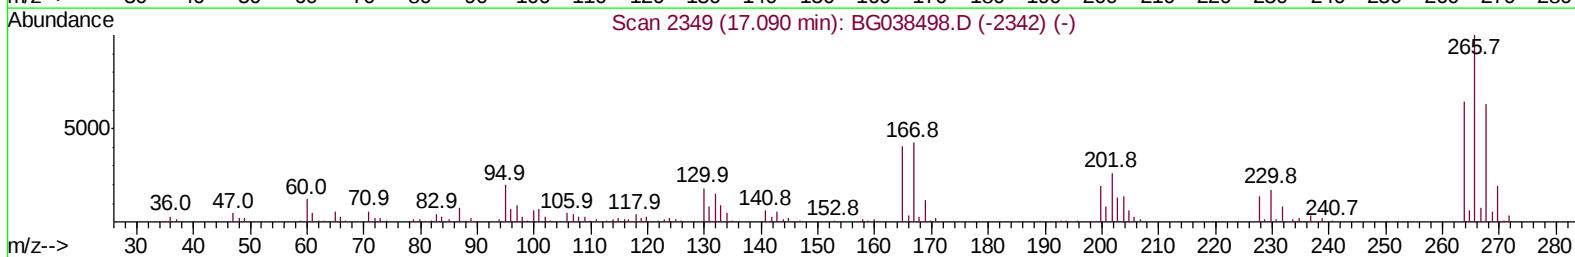
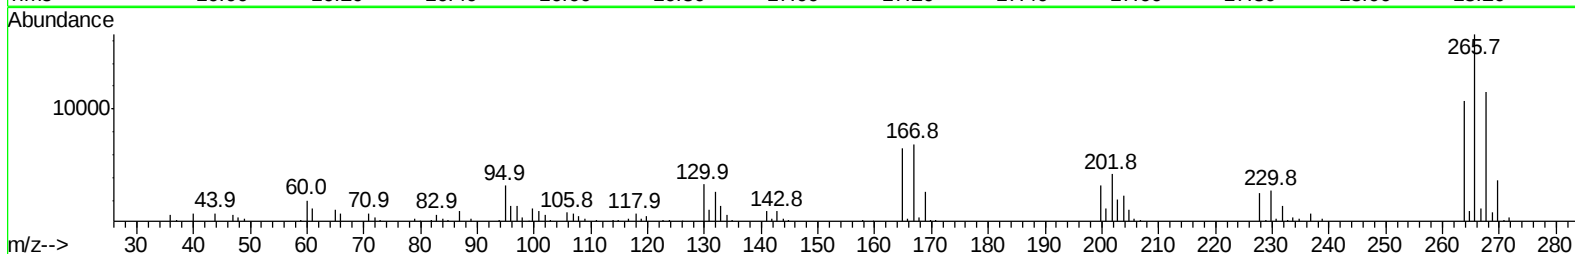


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121318\
Data File : BG038554.D
Acq On : 14 Dec 2018 5:13
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 08:53:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

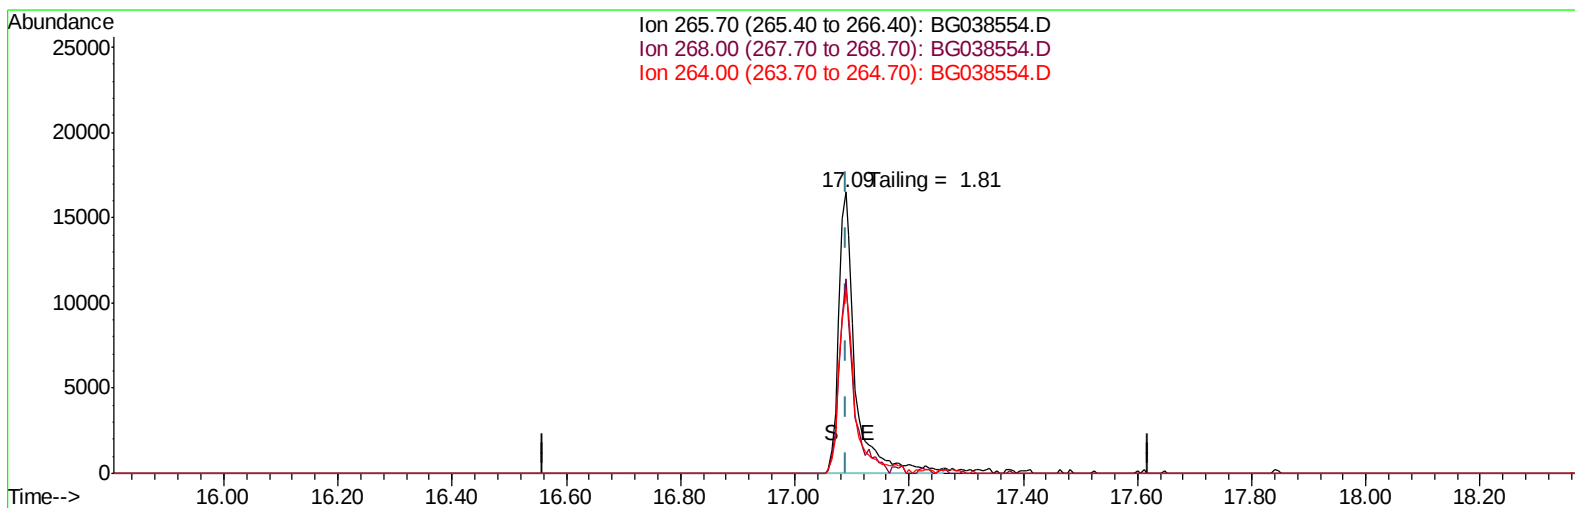

TIC: BG038554.D

(70) Pentachlorophenol (C)




17.089min (-0.002) 24393.83ng

response 32880

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	74.92
264.00	70.90	71.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121318\
Data File : BG038554.D
Acq On : 14 Dec 2018 5:13
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 08:53:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

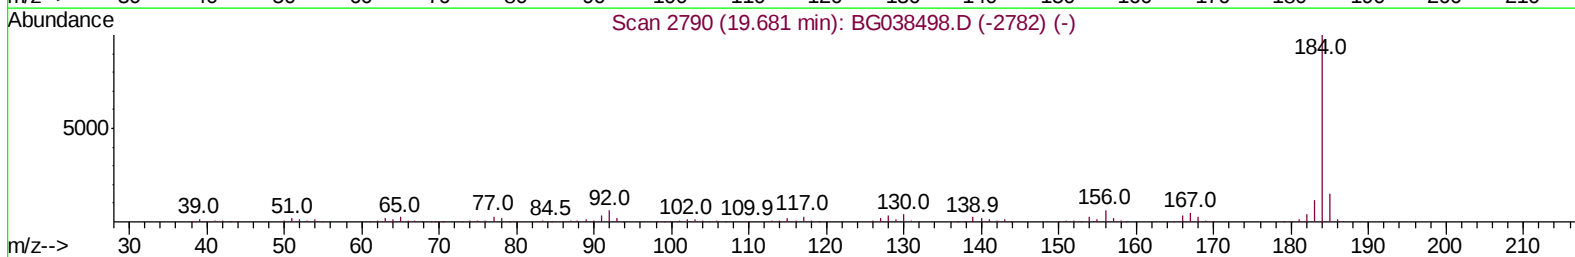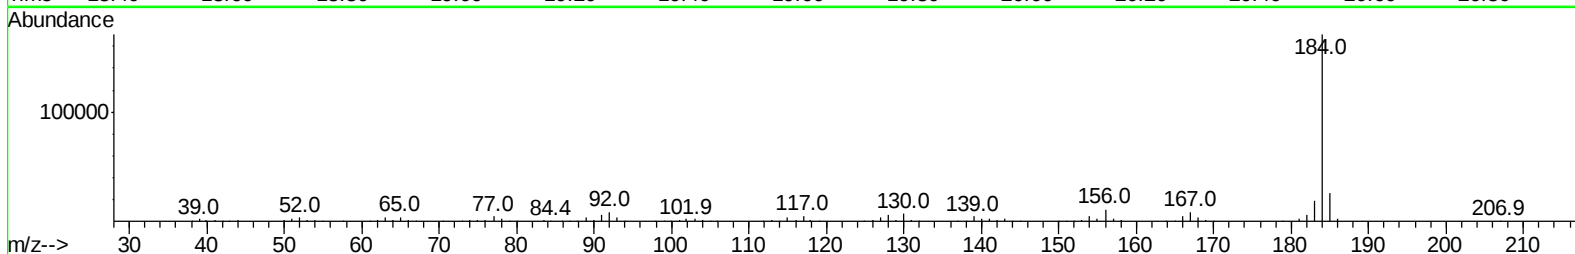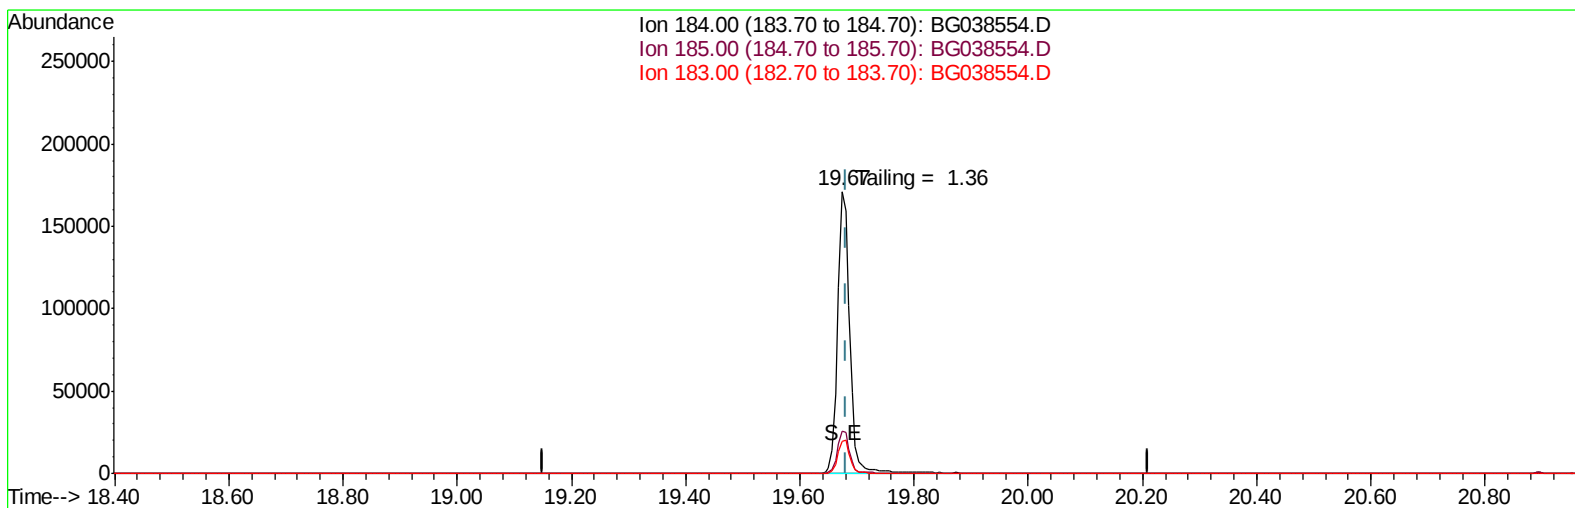

TIC: BG038554.D

(77) Benzidine

19.674min (-0.008) 0.00ng

response 249975

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.91
183.00	12.00	11.38
0.00	0.00	0.00