

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG121318\
Data File : BG038553.D
Acq On : 14 Dec 2018 4:34
Operator : JU/SJ
Sample : MECL2
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MECL2

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	8.059	840	846	856	rVB	59009	104623	27.43%	5.696%
2	10.879	1319	1326	1339	rBV	79251	150233	39.38%	8.180%
3	14.698	1967	1976	1987	rBV2	136340	240235	62.98%	13.080%
4	17.442	2436	2443	2452	rBV2	203976	325953	85.45%	17.747%
5	20.597	2975	2980	2987	rBV2	202849	251422	65.91%	13.689%
6	21.719	3164	3171	3182	rBV	222169	381465	100.00%	20.770%
7	23.993	3549	3558	3559	rBV9	2454	5178	1.36%	0.282%
8	25.009	3713	3731	3746	rBV2	128167	377543	98.97%	20.556%


Sum of corrected areas: 1836652

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG121318\
Data File : BG038553.D
Acq On : 14 Dec 2018 4:34
Operator : JU/SJ
Sample : MECL2
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MECL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

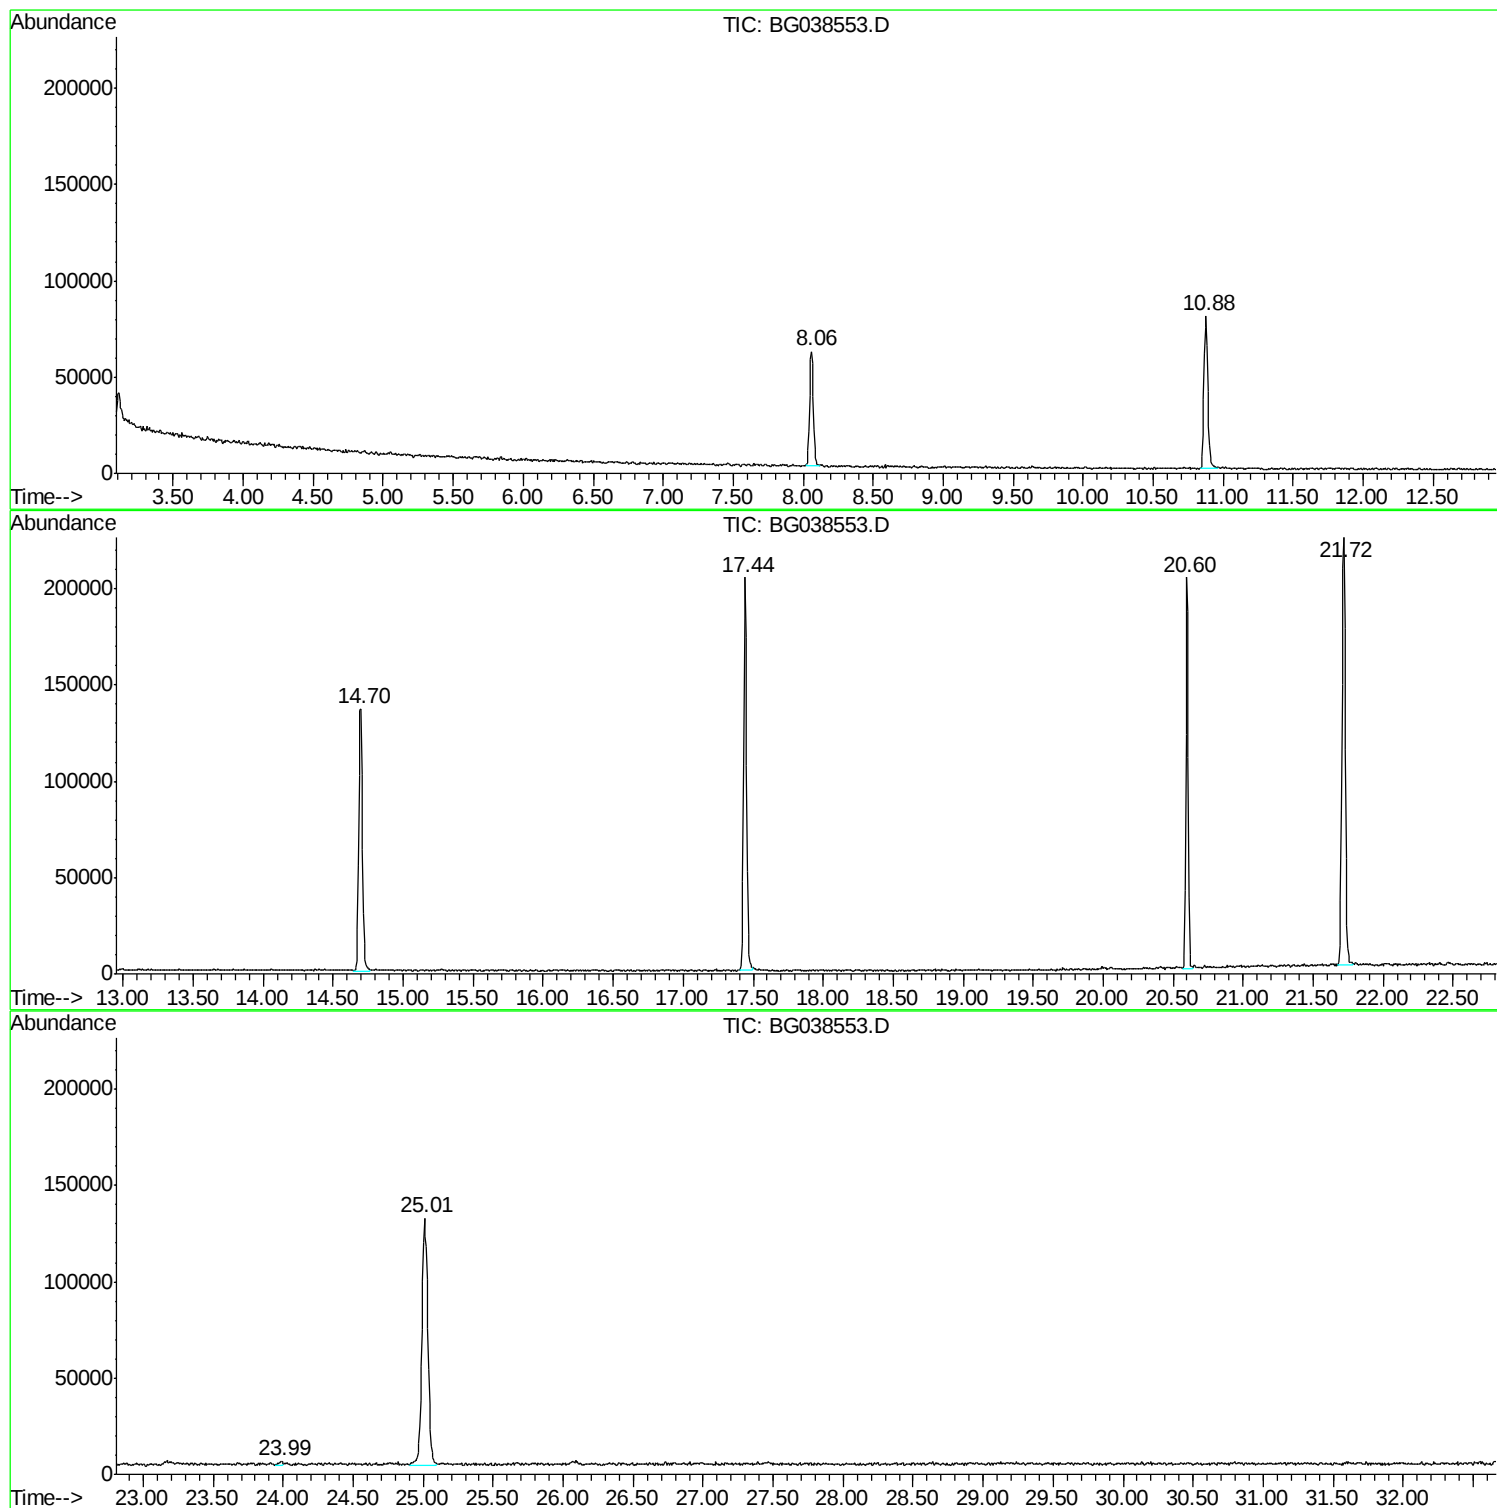

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG121318\
Data File : BG038553.D
Acq On : 14 Dec 2018 4:34
Operator : JU/SJ
Sample : MECL2
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MECL2










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown20.60 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.60	13.18 ng	251422	Chrysene-d12	21.72

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1H-Cyclopenta[1,2-c:3,4-c']difur...	210	C9H6O6	006053-68-5	12
2		Propanedinitrile	66	C3H2N2	000109-77-3	12
3		Dimethyl-5-norbornene-2,3-dicarb...	210	C11H14O4	005826-73-3	10
4		4-Hydroxy-4-azatricyclo[5.2.1.0(...	179	C9H9NO3	1000210-21-2	10
5		3-Butenenitrile, 3-chloro-	101	C4H4ClN	021031-46-9	10

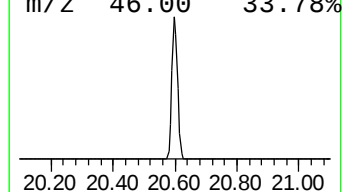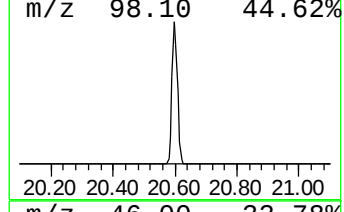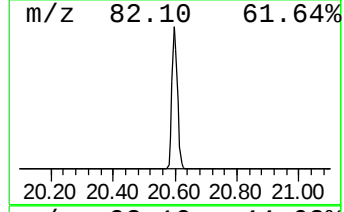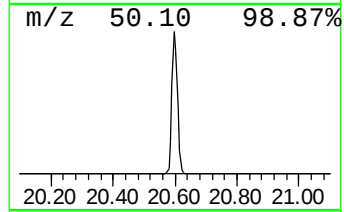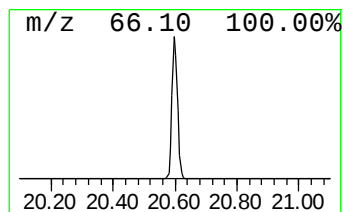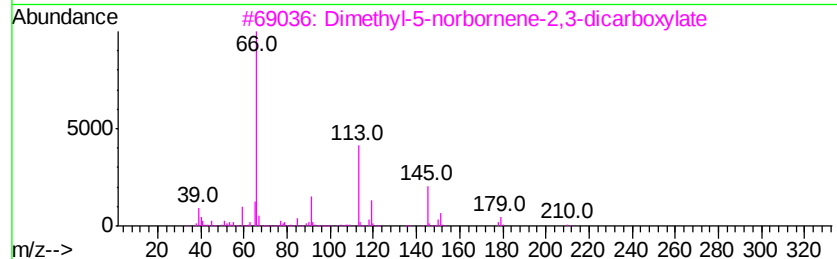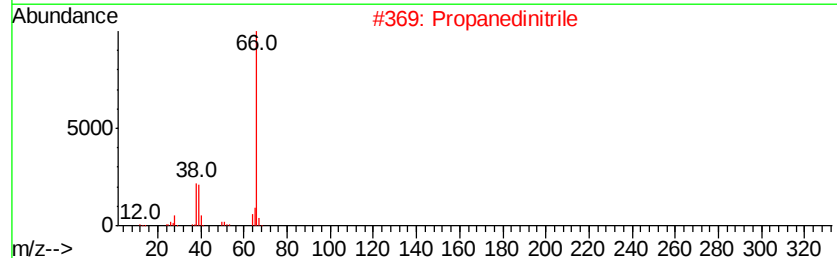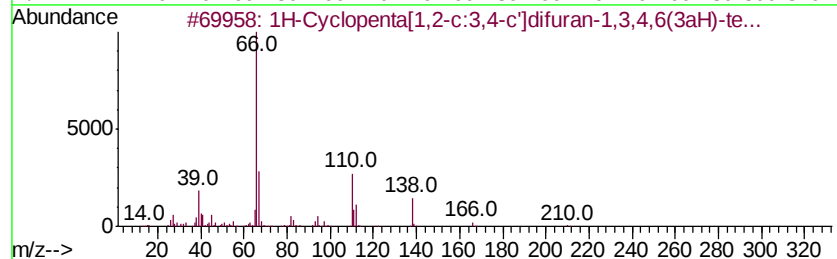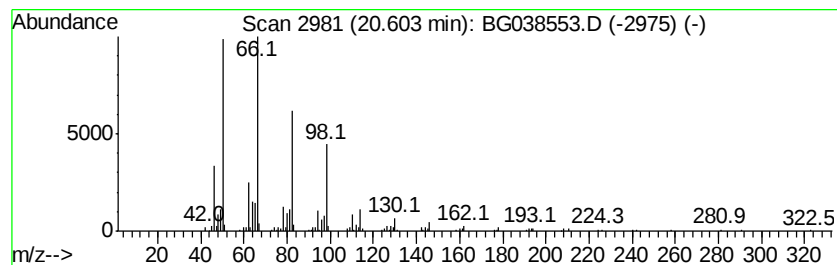

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG121318\
Data File : BG038553.D
Acq On : 14 Dec 2018 4:34
Operator : JU/SJ
Sample : MECL2
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MECL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown20.60	20.60	13.2	ng	251422	5	21.72	381465	20.0