


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121318\
 Data File : BG038535.D
 Acq On : 13 Dec 2018 16:46
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

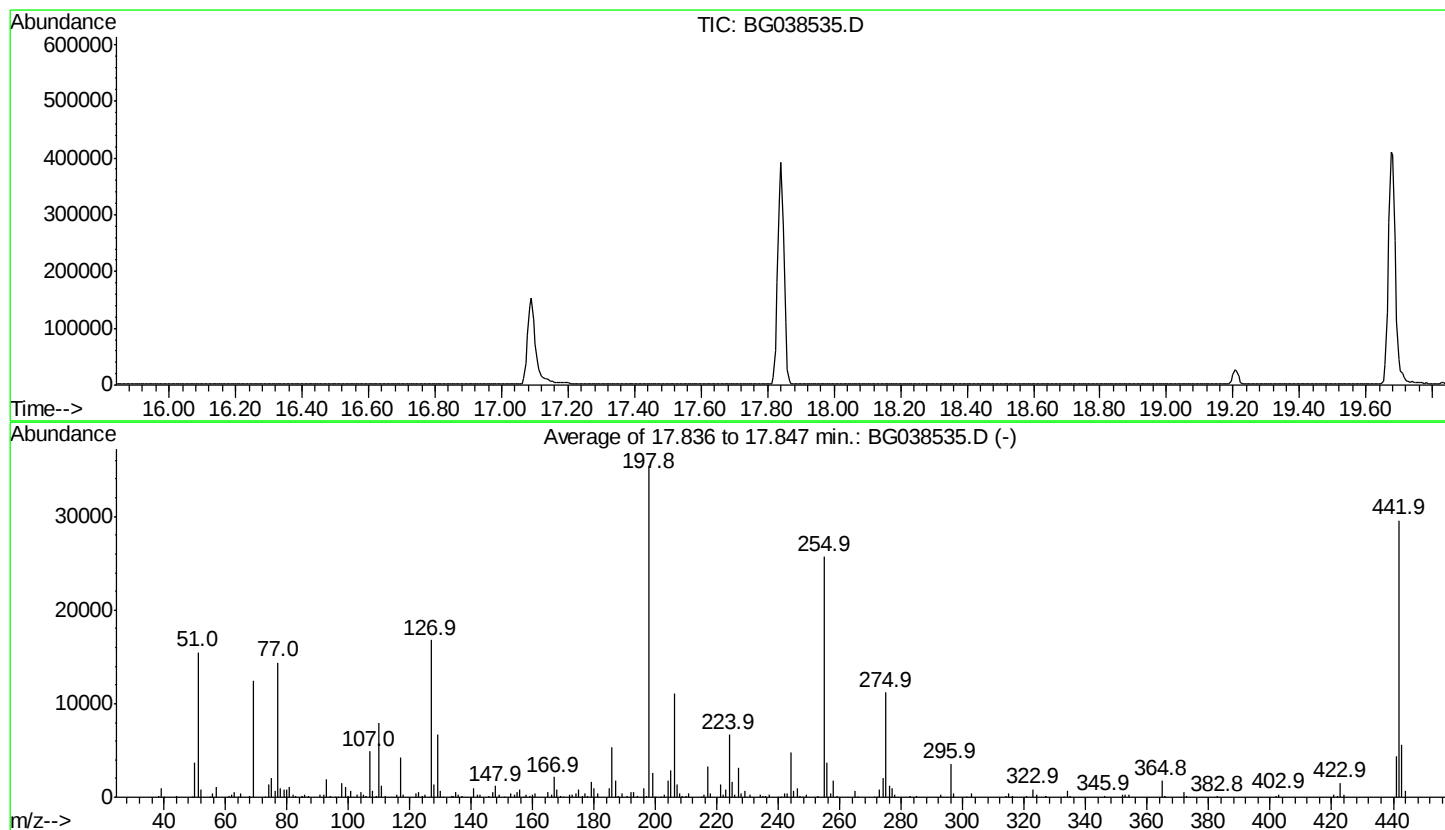

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.8	15519	PASS
68	69	0.00	2	1.4	170	PASS
69	198	0.00	100	35.1	12444	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.3	16764	PASS
197	198	0.00	2	0.4	136	PASS
198	198	100	100	100.0	35434	PASS
199	198	5	9	7.2	2542	PASS
275	198	10	60	31.5	11173	PASS
365	198	1	100	5.0	1757	PASS
441	198	0.01	100	12.2	4322	PASS
442	198	50	100	83.6	29608	PASS
443	442	15	24	19.2	5679	PASS