


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121318\
 Data File : BG038554.D
 Acq On : 14 Dec 2018 5:13
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

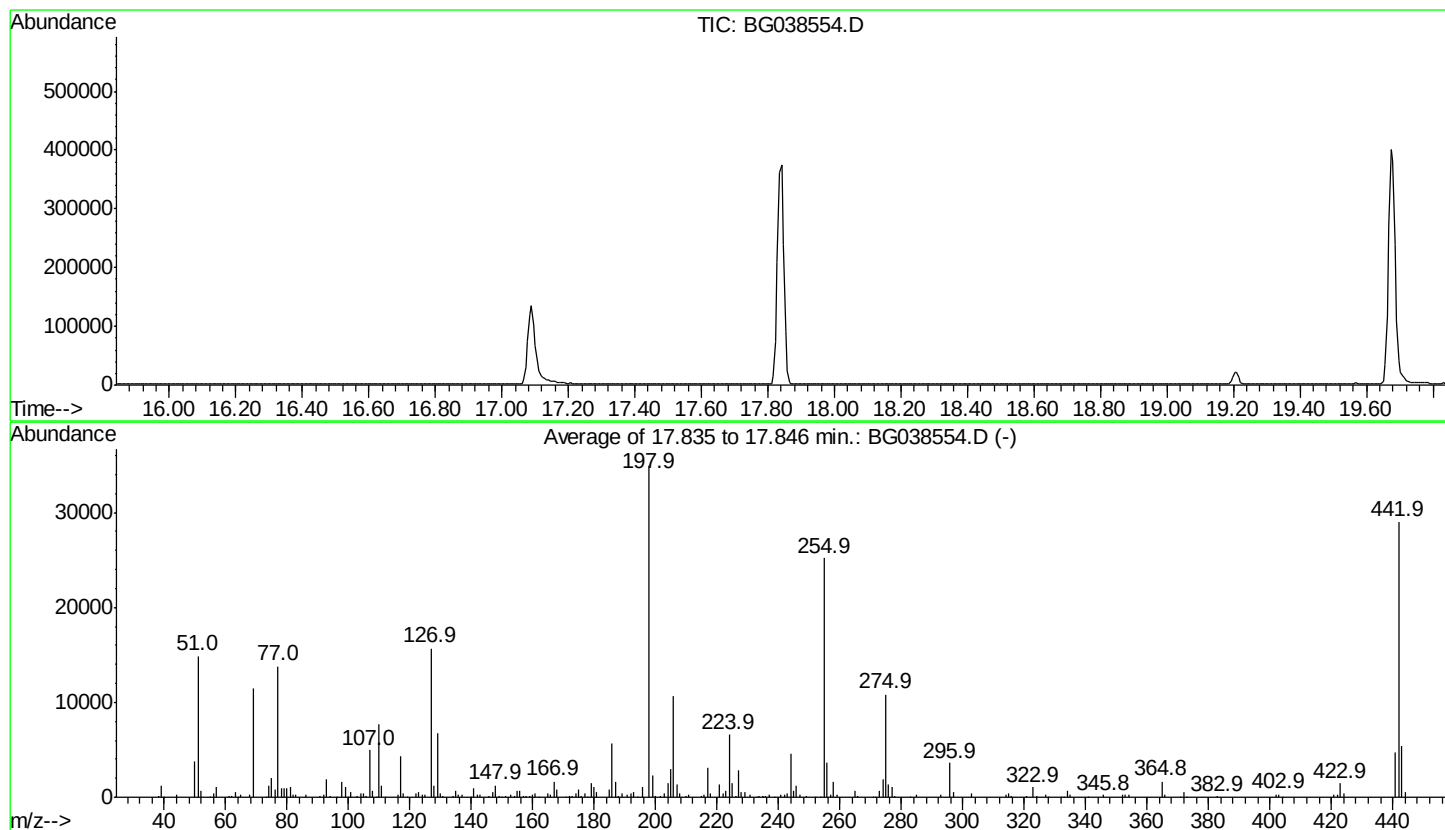

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	14846	PASS
68	69	0.00	2	2.0	233	PASS
69	198	0.00	100	33.0	11533	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.9	15689	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	34946	PASS
199	198	5	9	6.7	2355	PASS
275	198	10	60	31.0	10845	PASS
365	198	1	100	4.7	1656	PASS
441	198	0.01	100	13.4	4679	PASS
442	198	50	100	83.1	29026	PASS
443	442	15	24	18.7	5420	PASS