
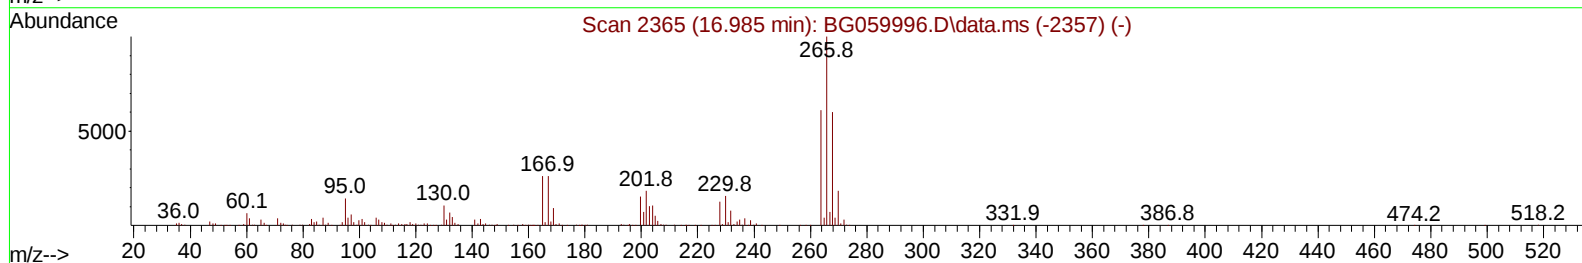
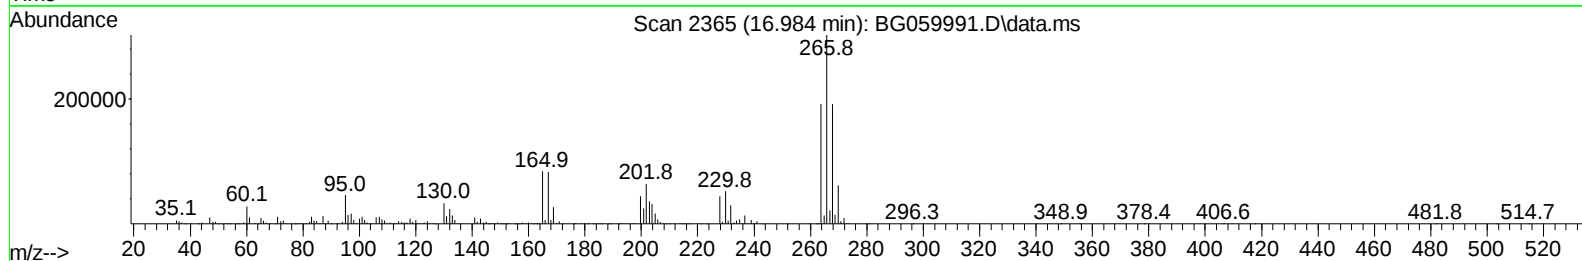


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121323\
Data File : BG059991.D
Acq On : 13 Dec 2023 10:08
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Dec 13 17:42:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 13 17:28:49 2023
Response via : Initial Calibration

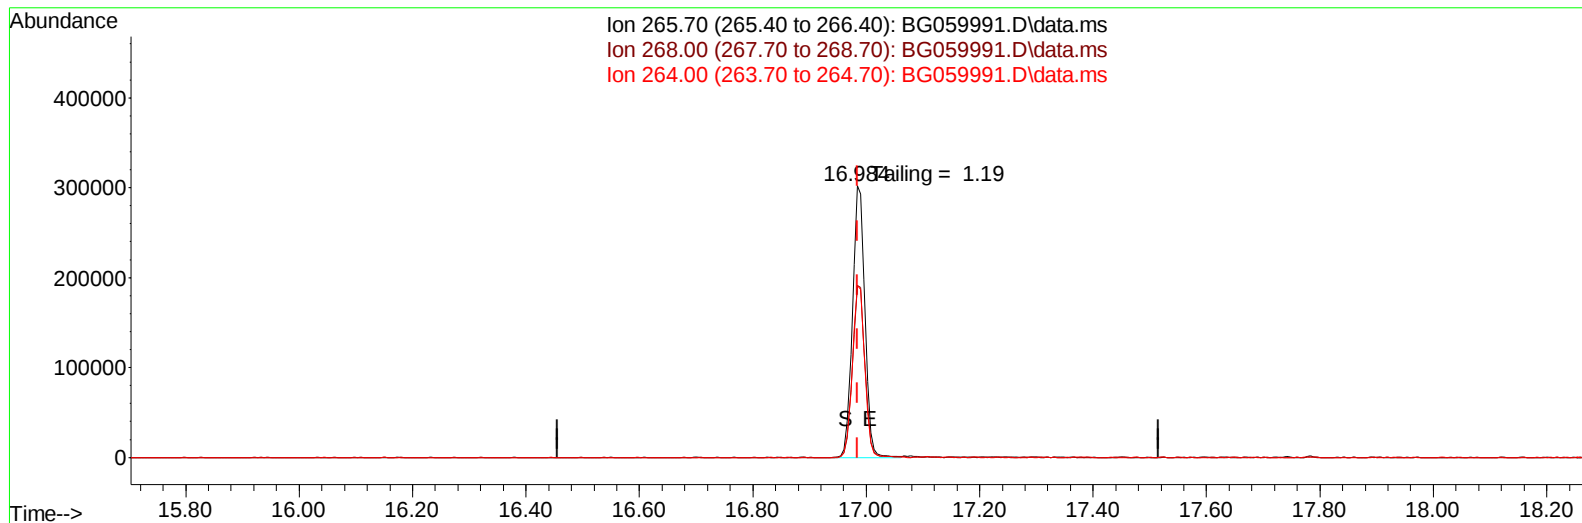




TIC: BG059991.D\data.ms

(70) Pentachlorophenol (C)**16.984min (-0.001) 104124.82 ng****response 461400**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	63.32
264.00	61.00	63.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121323\
Data File : BG059991.D
Acq On : 13 Dec 2023 10:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Dec 13 17:42:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 13 17:28:49 2023
Response via : Initial Calibration

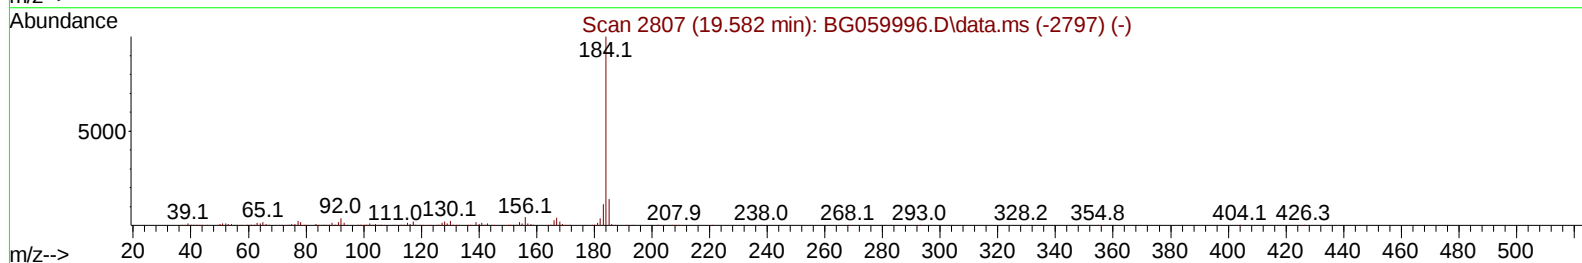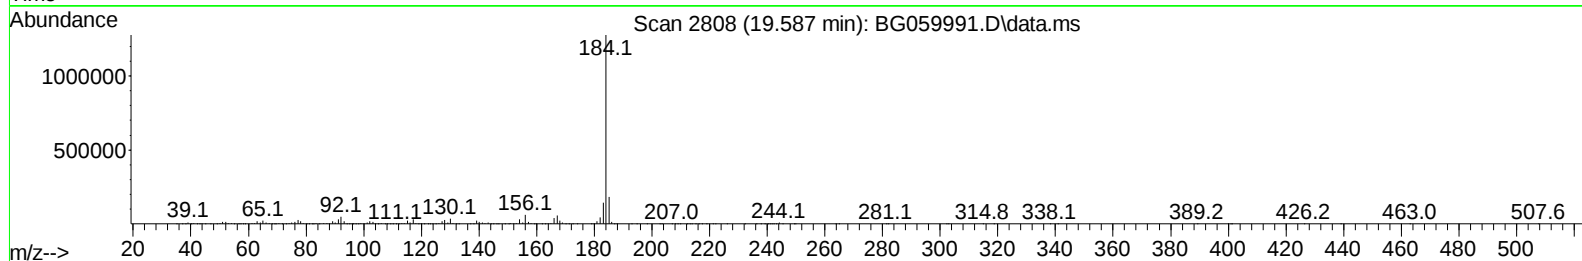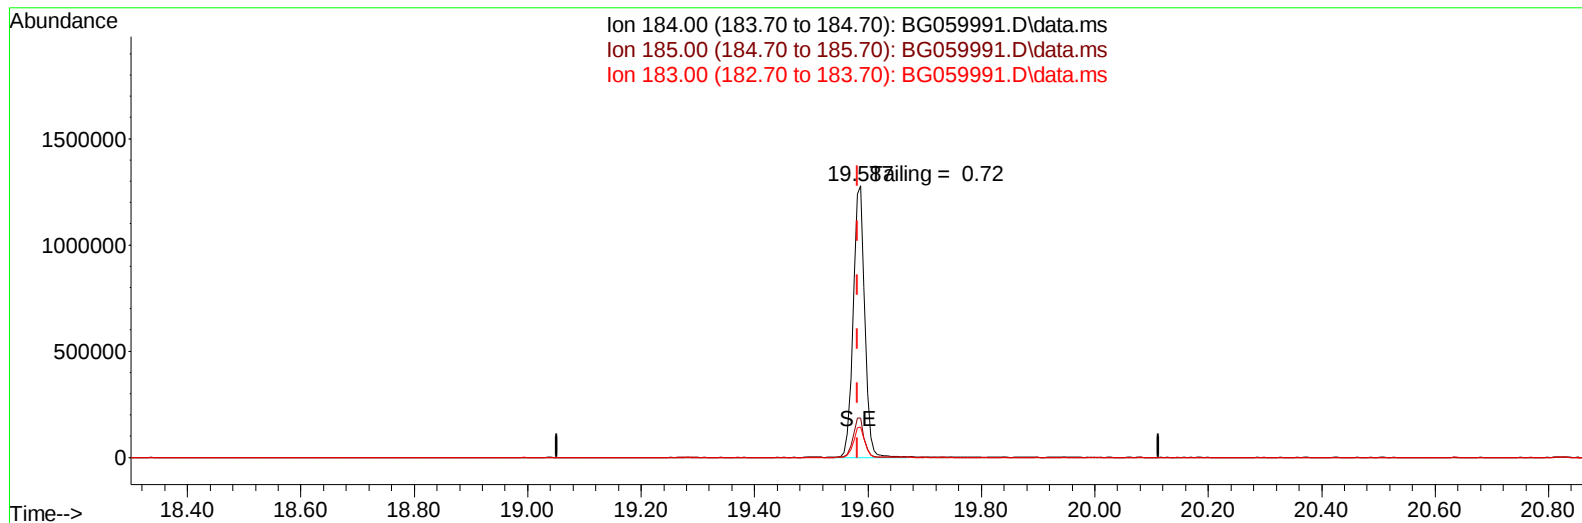

TIC: BG059991.D\data.ms

(77) Benzidine**19.587min (+ 0.005) 49138.67 ng****response 1818032**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.42
183.00	11.20	11.14
0.00	0.00	0.00