

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121323\
Data File : BG060001.D
Acq On : 13 Dec 2023 18:04
Operator : MA/JU
Sample : PB157563BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157563BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060001.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.522	407	414	424	rBV	651733	989043	8.25%	3.253%
2	7.109	677	684	693	rBV	898387	1464949	12.21%	4.819%
3	7.955	822	828	835	rVB	218070	352633	2.94%	1.160%
4	9.112	1017	1025	1033	rBV	505250	876728	7.31%	2.884%
5	10.757	1297	1305	1313	rBV	283971	502359	4.19%	1.652%
6	13.219	1716	1724	1731	rBV	2313463	3552706	29.62%	11.686%
7	14.594	1951	1958	1964	rBV	517705	809857	6.75%	2.664%
8	16.081	2203	2211	2224	rBV	3299379	4682432	39.04%	15.402%
9	17.338	2419	2425	2433	rBV	869019	1277127	10.65%	4.201%
10	19.964	2865	2872	2881	rBV	9036966	11993713	100.00%	39.450%
11	21.609	3144	3152	3158	rBV2	1186927	1886604	15.73%	6.206%
12	24.800	3682	3695	3706	rBV	692183	2013946	16.79%	6.624%




Sum of corrected areas: 30402097

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121323\
Data File : BG060001.D
Acq On : 13 Dec 2023 18:04
Operator : MA/JU
Sample : PB157563BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157563BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

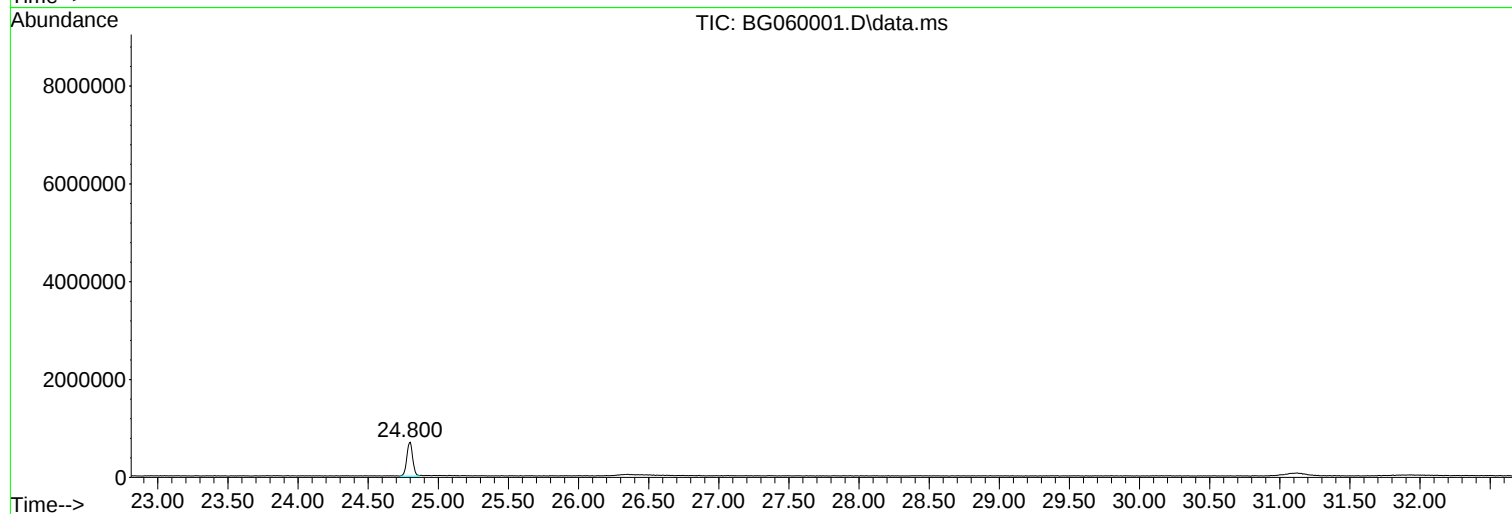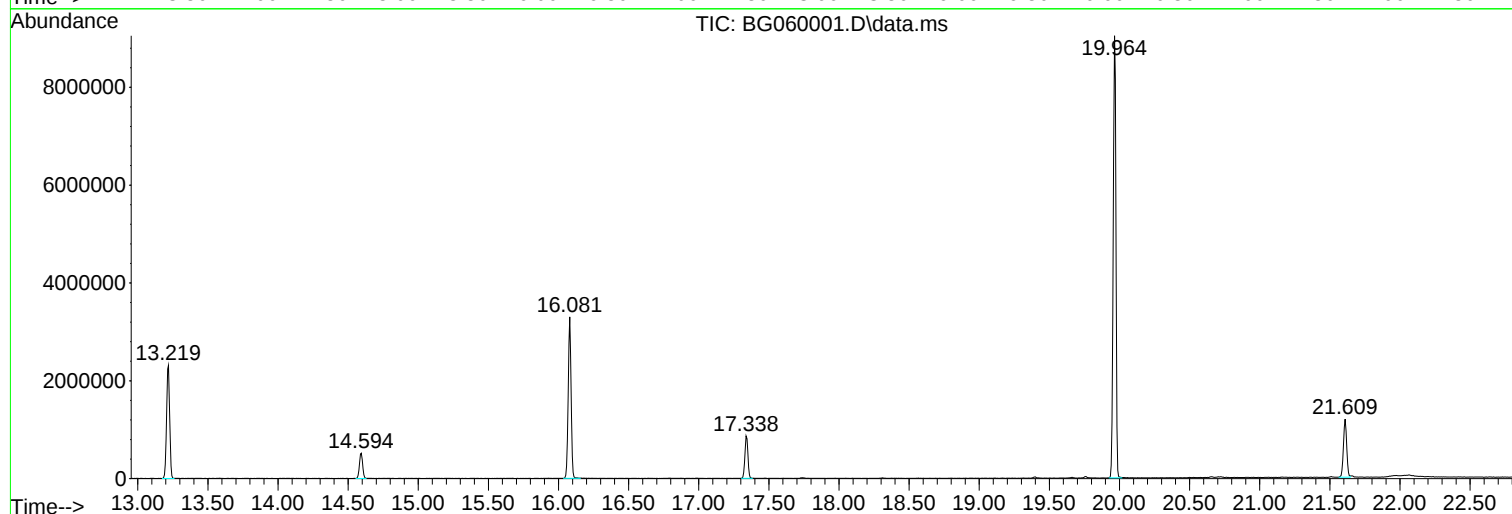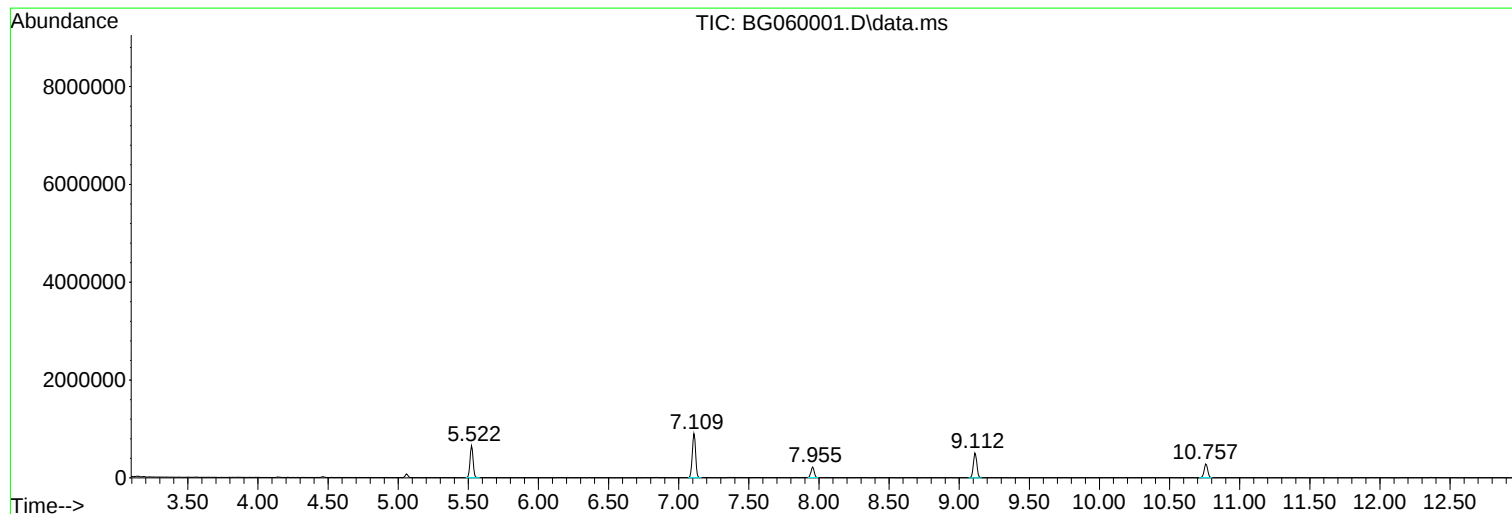

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121323\
Data File : BG060001.D
Acq On : 13 Dec 2023 18:04
Operator : MA/JU
Sample : PB157563BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157563BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121323\
Data File : BG060001.D
Acq On : 13 Dec 2023 18:04
Operator : MA/JU
Sample : PB157563BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157563BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------