


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG121323\  
Data File : BG059991.D  
Acq On : 13 Dec 2023 10:08  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG121323.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Dec 14 01:47:12 2023

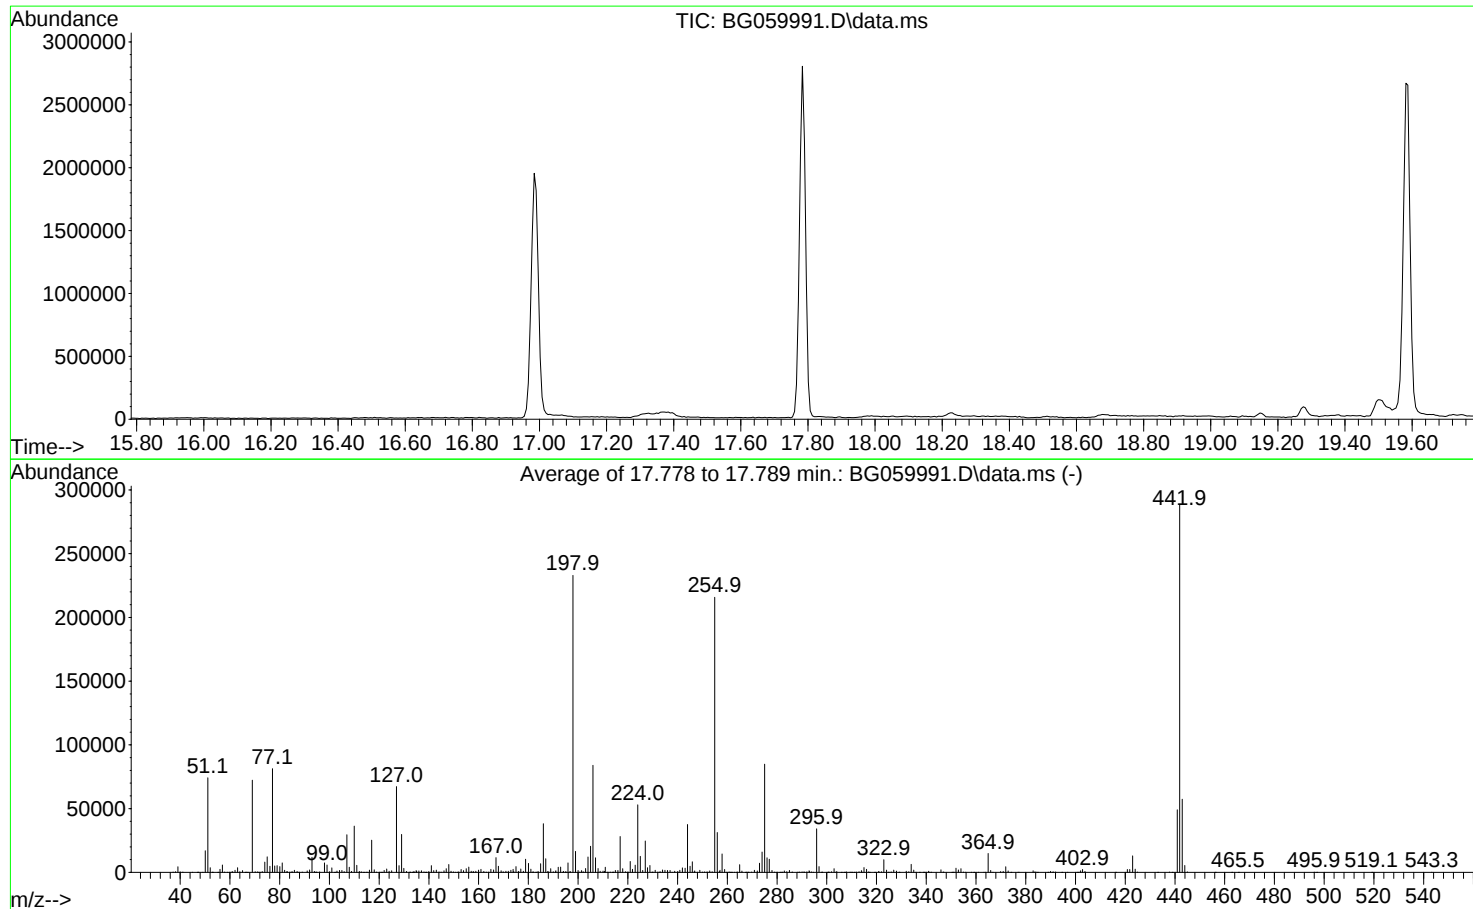




AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2493

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 51     | 198     | 10     | 80     | 31.9  | 74229  | PASS      |
| 68     | 69      | 0.00   | 2      | 0.0   | 0      | PASS      |
| 69     | 198     | 0.00   | 100    | 31.0  | 72275  | PASS      |
| 70     | 69      | 0.00   | 2      | 0.7   | 476    | PASS      |
| 127    | 198     | 10     | 80     | 28.9  | 67283  | PASS      |
| 197    | 198     | 0.00   | 2      | 0.2   | 554    | PASS      |
| 198    | 198     | 100    | 100    | 100.0 | 233045 | PASS      |
| 199    | 198     | 5      | 9      | 7.0   | 16415  | PASS      |
| 275    | 198     | 10     | 60     | 36.4  | 84805  | PASS      |
| 365    | 198     | 1      | 100    | 6.4   | 14879  | PASS      |
| 441    | 198     | 0.01   | 100    | 21.1  | 49131  | PASS      |
| 442    | 442     | 50     | 100    | 100.0 | 288597 | PASS      |
| 443    | 442     | 15     | 24     | 19.9  | 57323  | PASS      |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG121323\  
Data File : BG059991.D  
Acq On : 13 Dec 2023 10:08  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Dec 13 17:42:32 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG121323.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 13 17:28:49 2023  
Response via : Initial Calibration

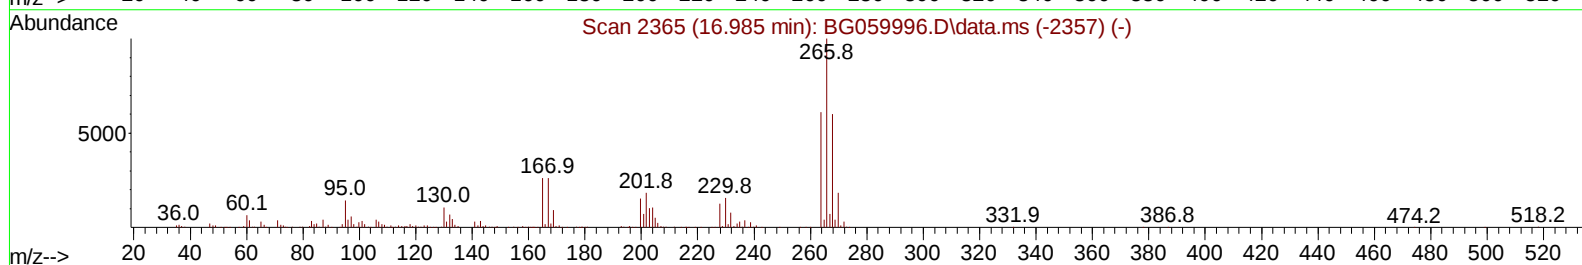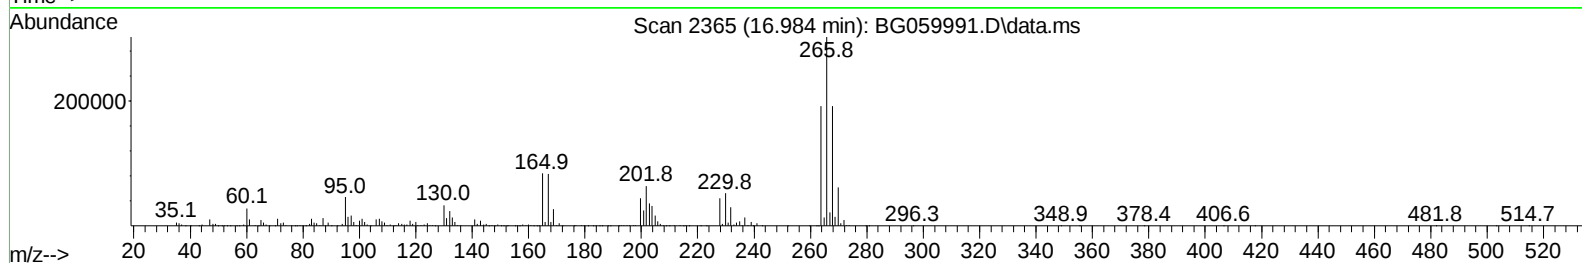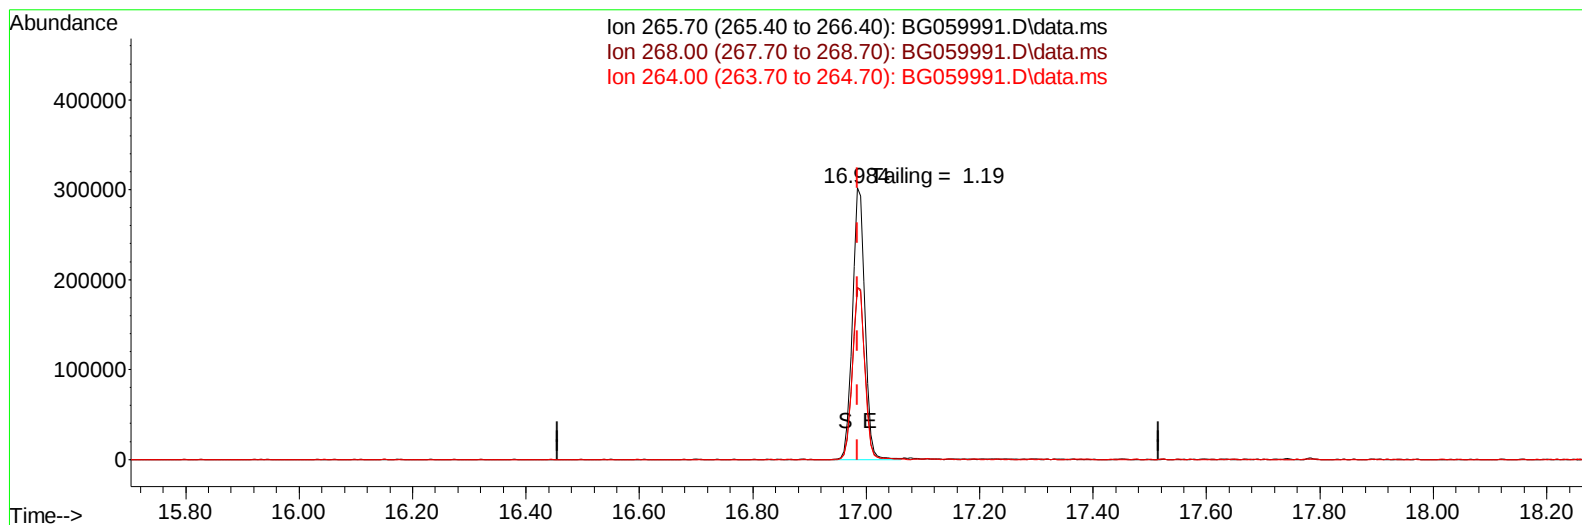

TIC: BG059991.D\data.ms

**(70) Pentachlorophenol (C)**

**16.984min (-0.001) 104124.82 ng**




**response 461400**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 59.90  | 63.32  |
| 264.00 | 61.00  | 63.34  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG121323\  
Data File : BG059991.D  
Acq On : 13 Dec 2023 10:08  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Dec 13 17:42:32 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG121323.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 13 17:28:49 2023  
Response via : Initial Calibration

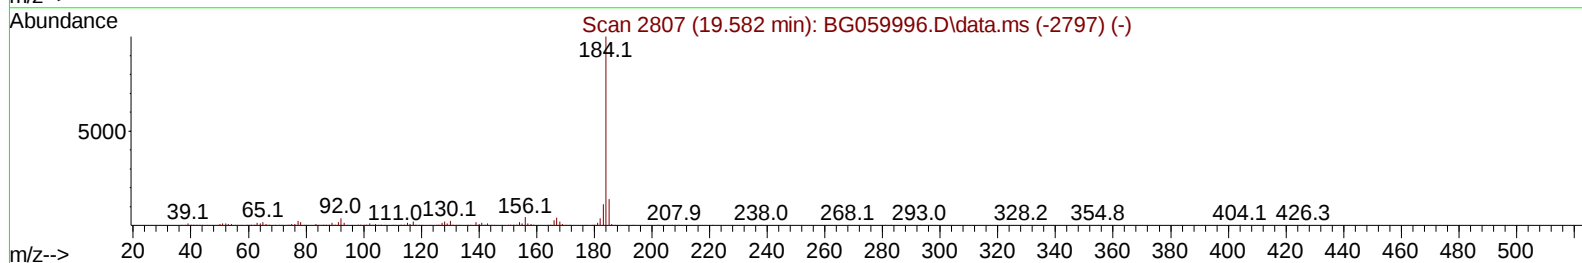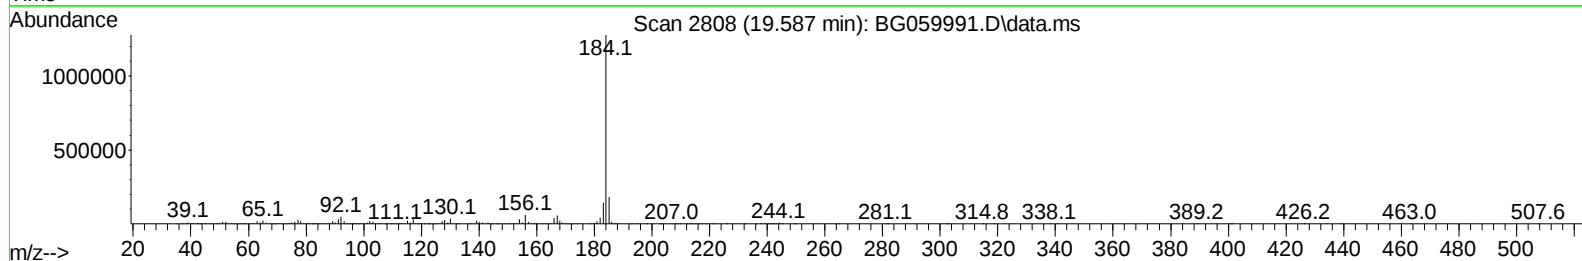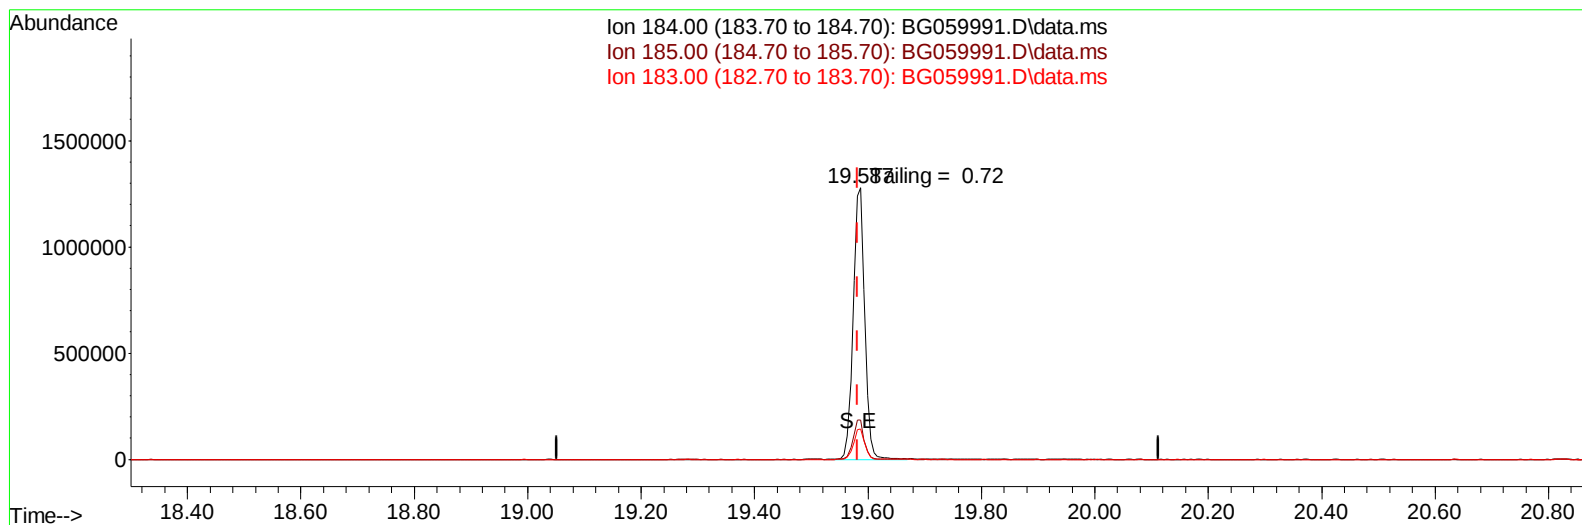

TIC: BG059991.D\data.ms

(77) Benzidine

19.587min (+ 0.005) 49138.67 ng

response 1818032

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.90  | 14.42  |
| 183.00 | 11.20  | 11.14  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 12/13/2023    | BNA_G            | <u>BG059991.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 847699           | 20.821             |
| DDD           | 17512            | 20.374             |
| DDE           | 0                | 19.898             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 17512         | 865211           | 2.02               |
|               |                  |                    |

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP