
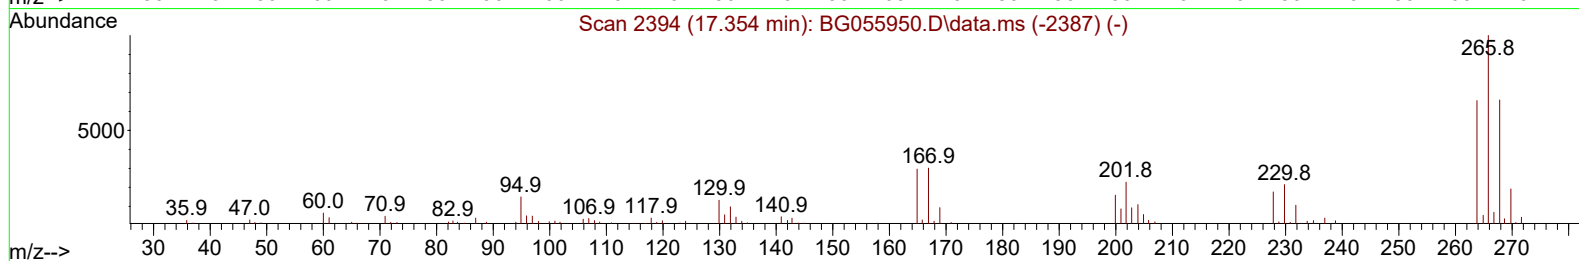
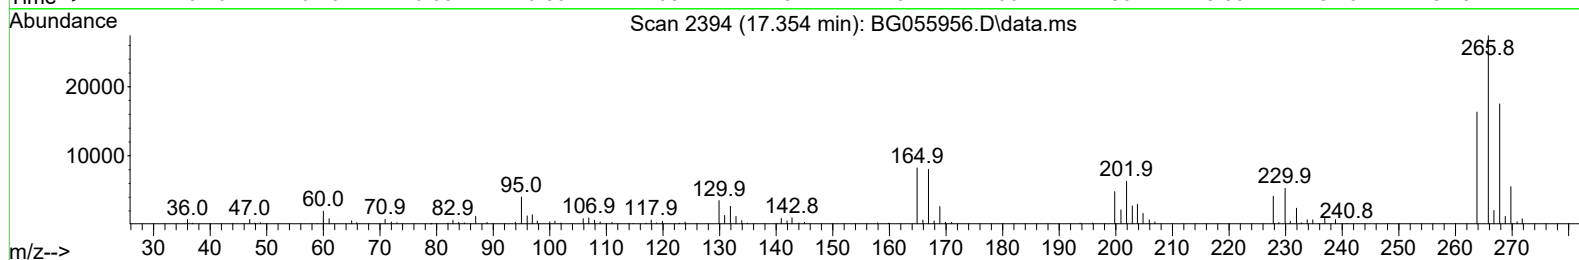


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121422\
Data File : BG055956.D
Acq On : 14 Dec 2022 12:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 05:37:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 14 02:24:06 2022
Response via : Initial Calibration

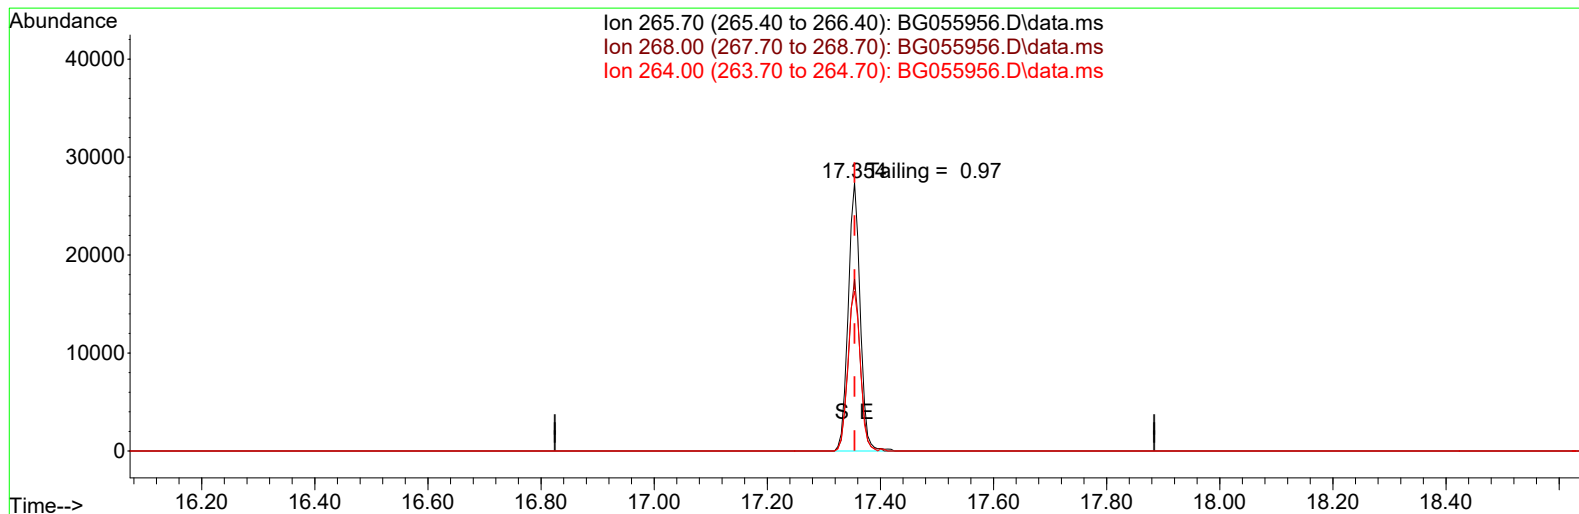

TIC: BG055956.D\data.ms

(70) Pentachlorophenol (C)




17.354min (-0.000) 22252.24 ng

response 40411

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.40	63.99
264.00	65.70	59.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121422\
Data File : BG055956.D
Acq On : 14 Dec 2022 12:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 05:37:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 14 02:24:06 2022
Response via : Initial Calibration

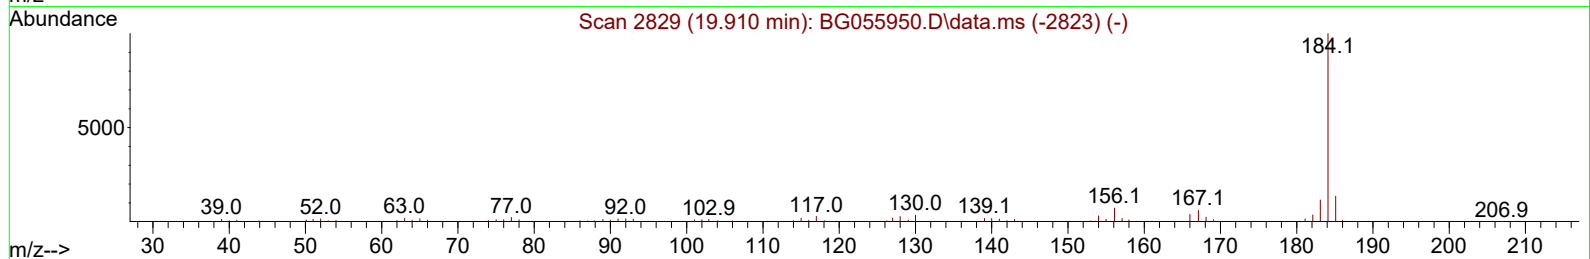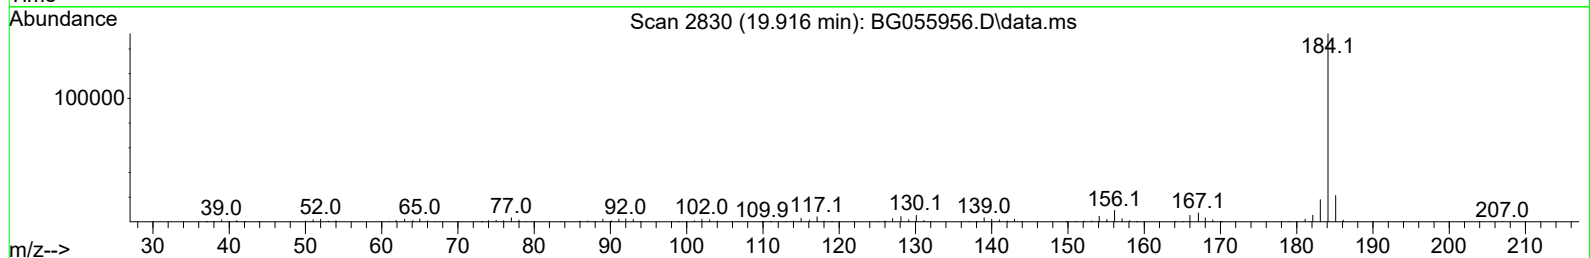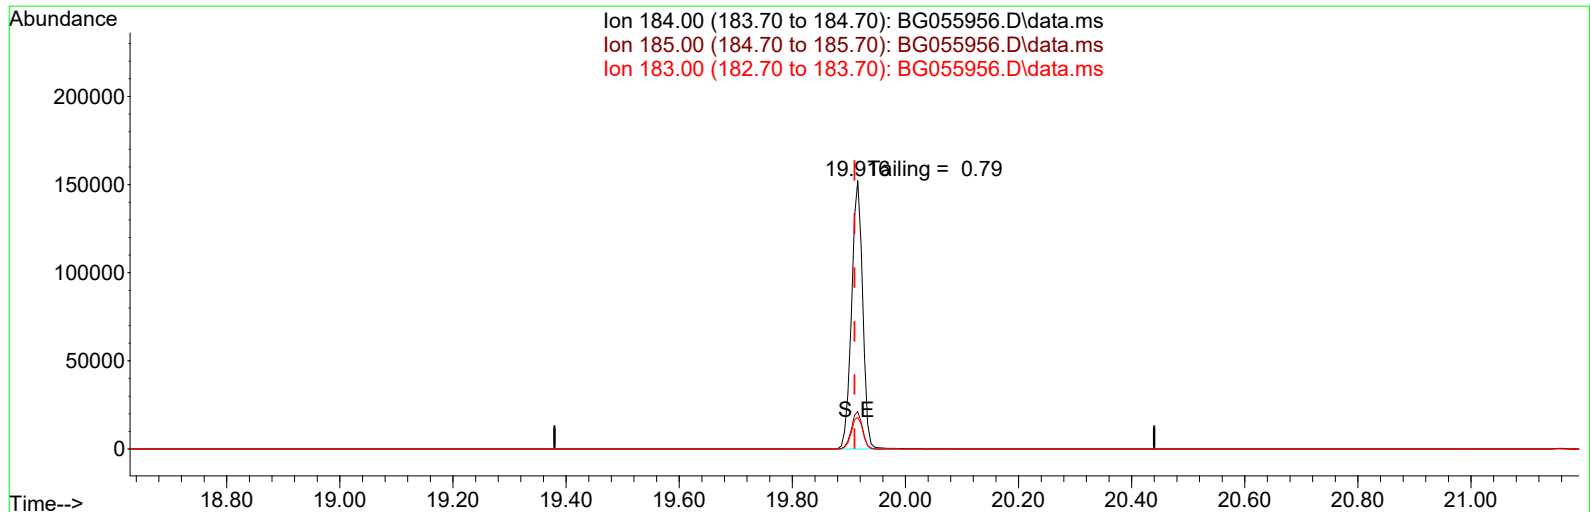

TIC: BG055956.D\data.ms

(77) Benzidine

19.916min (+ 0.006) 26653.27 ng

response 208294

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.05
183.00	11.50	11.83
0.00	0.00	0.00