


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121422\
 Data File : BG055956.D
 Acq On : 14 Dec 2022 12:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 14 02:24:06 2022

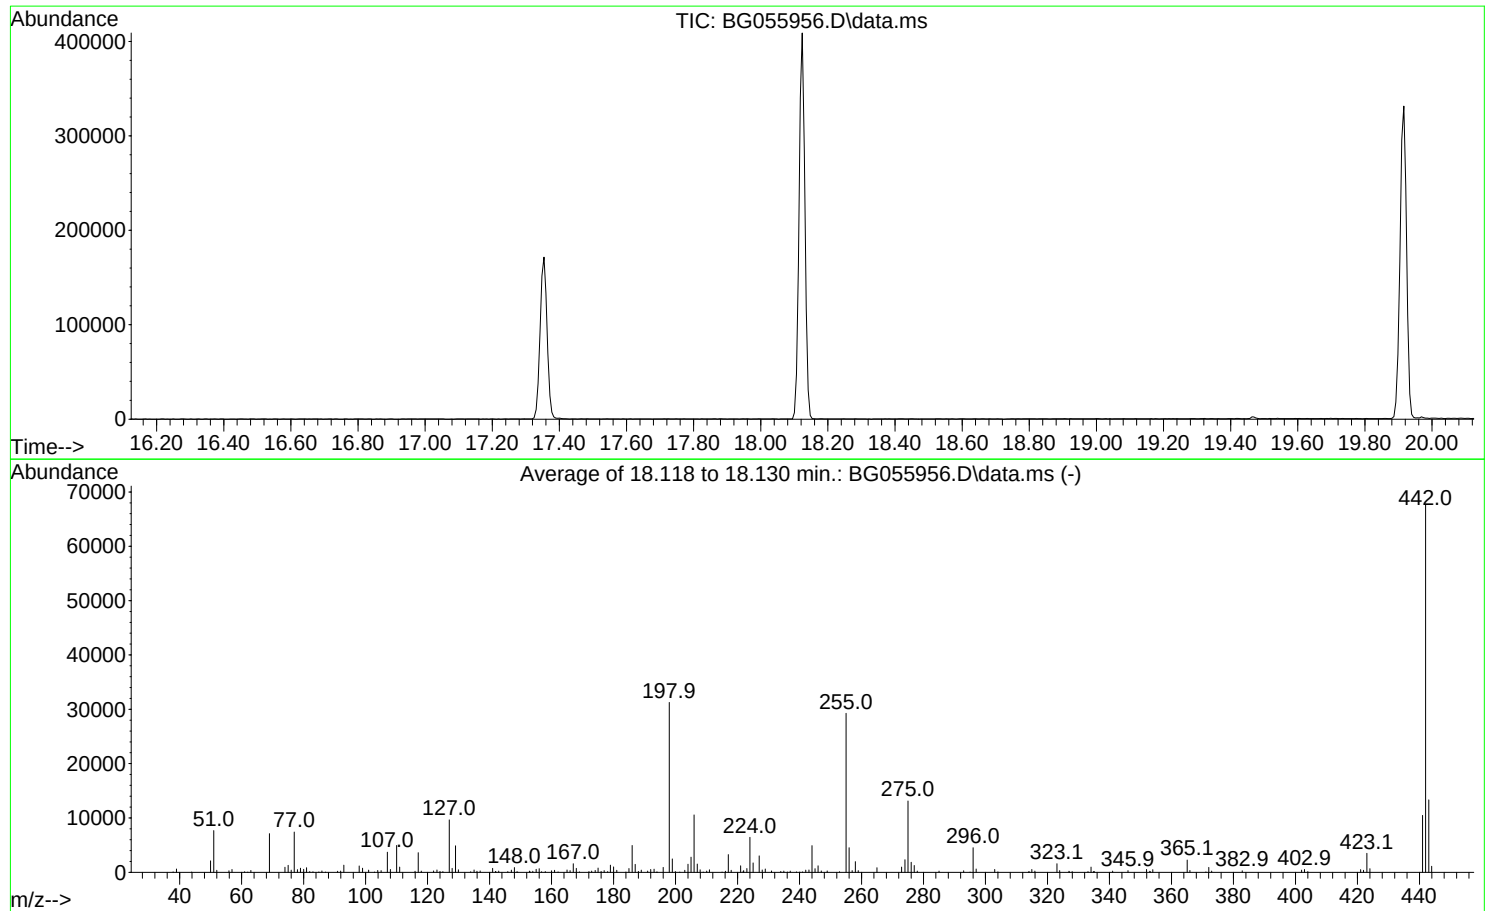




AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.5	7671	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	22.8	7114	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	30.9	9659	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31264	PASS
199	198	5	9	7.8	2452	PASS
275	198	10	60	42.0	13123	PASS
365	198	1	100	7.2	2254	PASS
441	198	0.01	100	33.5	10487	PASS
442	442	50	100	100.0	67707	PASS
443	442	15	24	19.7	13334	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121422\
Data File : BG055956.D
Acq On : 14 Dec 2022 12:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 15 05:37:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 14 02:24:06 2022
Response via : Initial Calibration

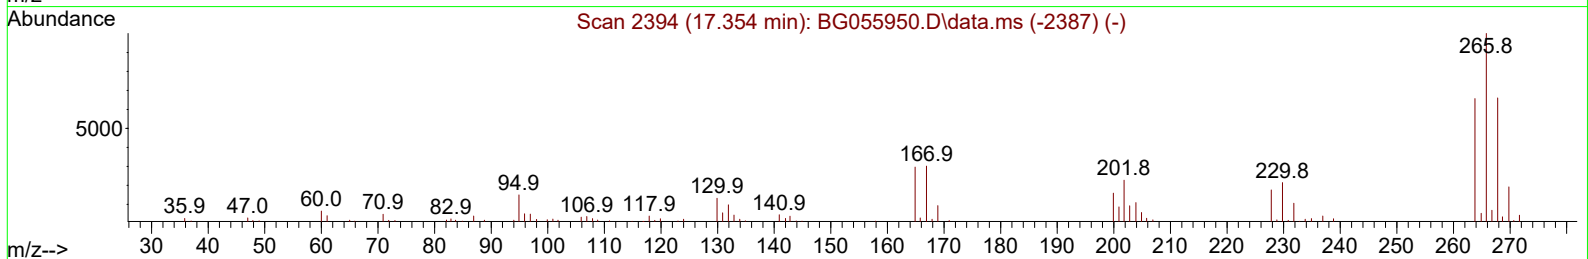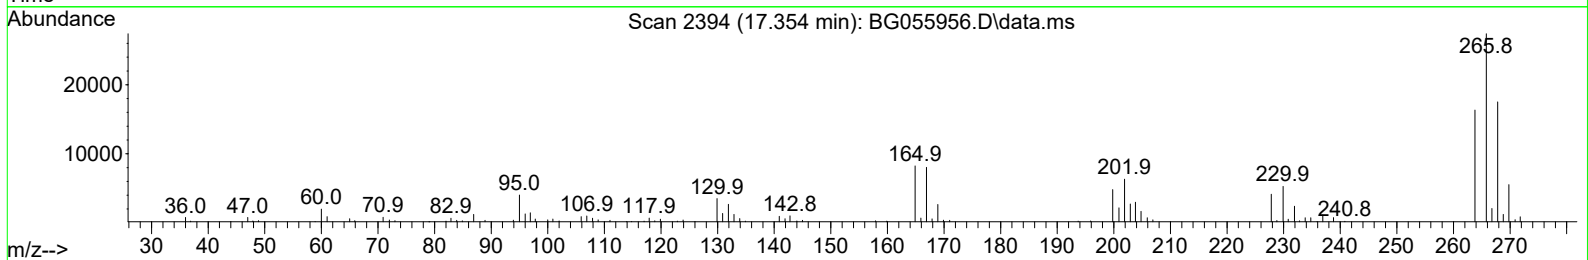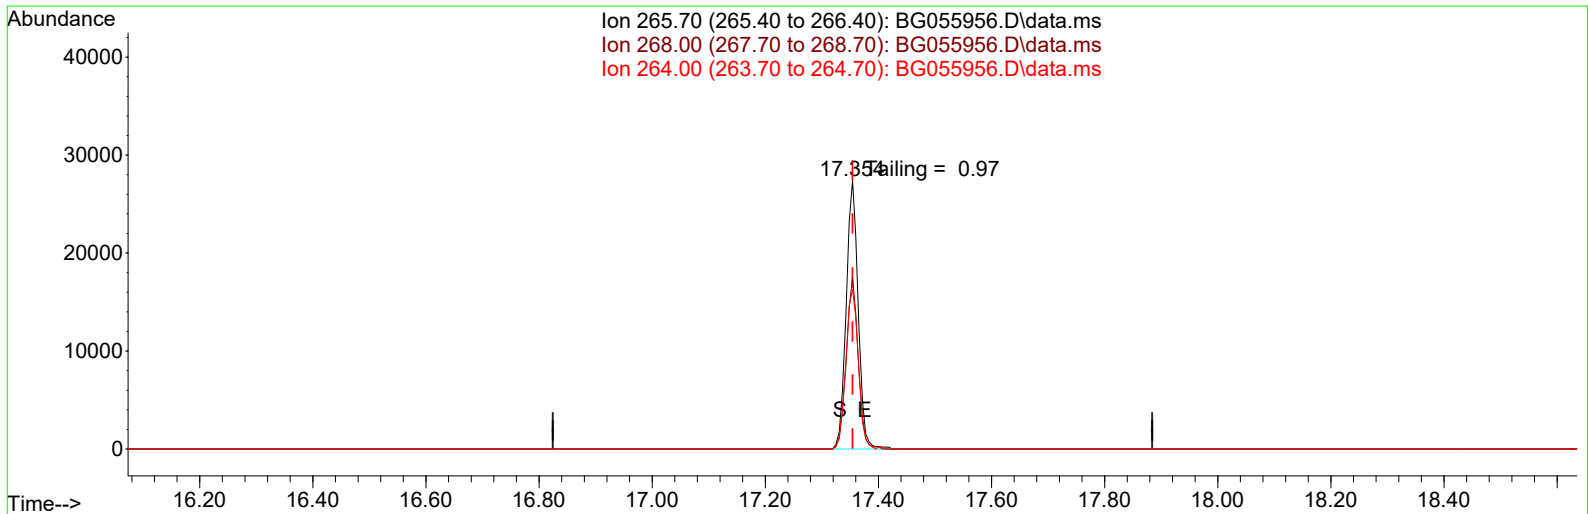

TIC: BG055956.D\data.ms

(70) Pentachlorophenol (C)

17.354min (-0.000) 22252.24 ng




response 40411

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.40	63.99
264.00	65.70	59.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121422\
Data File : BG055956.D
Acq On : 14 Dec 2022 12:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 15 05:37:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 14 02:24:06 2022
Response via : Initial Calibration

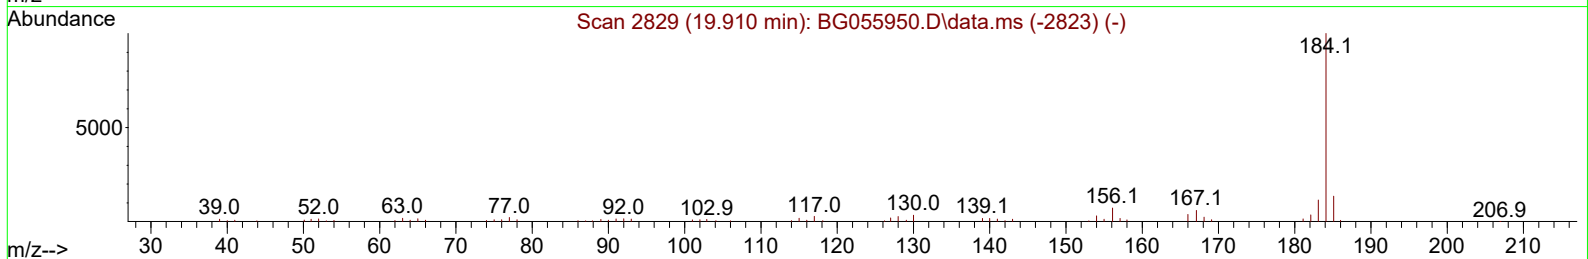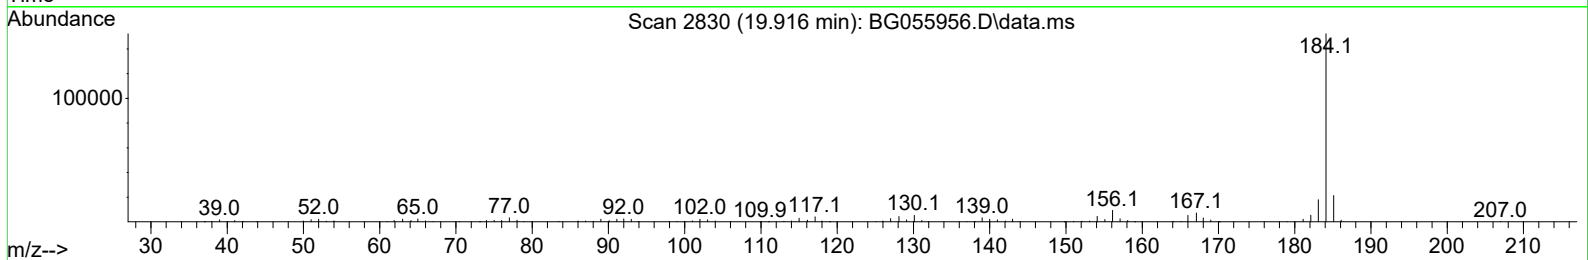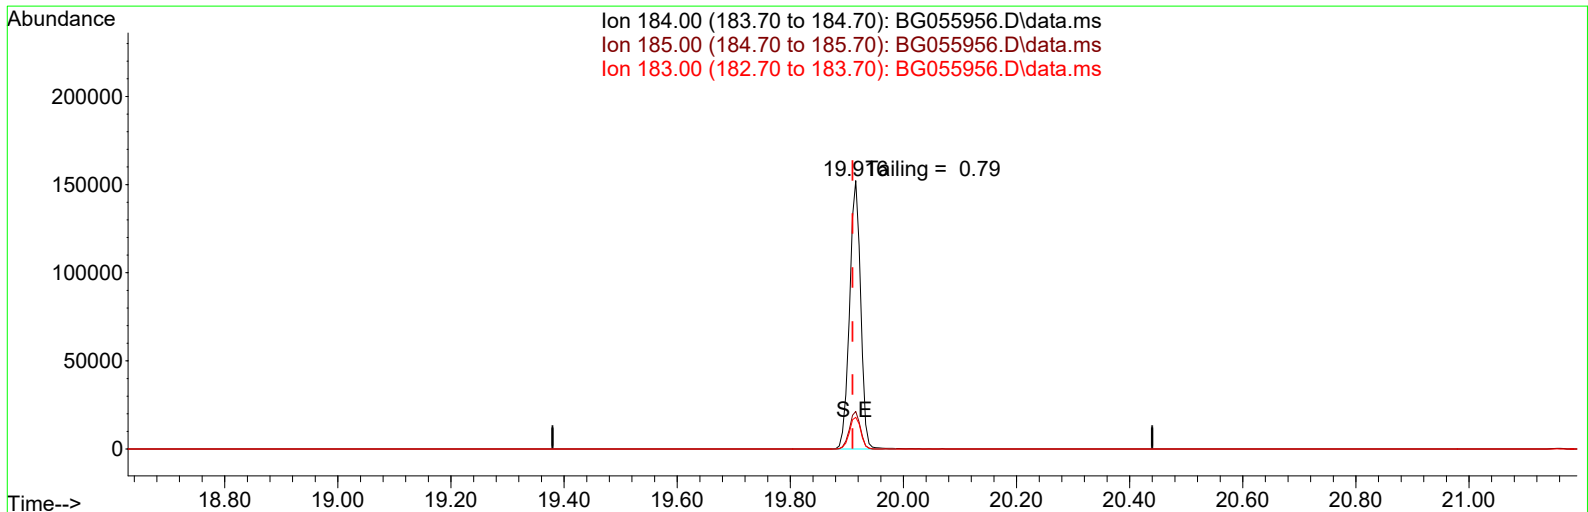

TIC: BG055956.D\data.ms

(77) Benzidine

19.916min (+ 0.006) 26653.27 ng

response 208294

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.05
183.00	11.50	11.83
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/14/2022	BNA_G	<u>BG055956.D</u>
Compound Name	Response	Retention Time
DDT	108684	21.161
DDD	2184	20.697
DDE	0	20.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2184	110868	1.97

Instrument :
BNA_G
ClientSampleId :
DFTPP