

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG121518\
 Data File : BG038612.D
 Acq On : 15 Dec 2018 20:06
 Operator : JU/SJ
 Sample : J6376-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TEST-PIT-1-WATER

Quant Time: Dec 16 04:06:16 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 12 15:26:27 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	23520	20.00	ng	0.00
21) Naphthalene-d8	10.88	136	94567	20.00	ng	0.00
39) Acenaphthene-d10	14.70	164	60434	20.00	ng	0.00
64) Phenanthrene-d10	17.44	188	151603	20.00	ng	0.00
76) Chrysene-d12	21.72	240	158143	20.00	ng	0.00
87) Perylene-d12	25.01	264	166019	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	77282	58.28	ng	0.00
7) Phenol-d6	7.21	99	63583	34.93	ng	0.00
23) Nitrobenzene-d5	9.24	82	172921	93.42	ng	0.00
42) 2,4,6-Tribromophenol	16.19	330	117221	140.74	ng	0.00
45) 2-Fluorobiphenyl	13.32	172	414191	94.02	ng	0.00
79) Terphenyl-d14	20.04	244	745139	102.54	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG121518\
Data File : BG038612.D
Acq On : 15 Dec 2018 20:06
Operator : JU/SJ
Sample : J6376-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TEST-PIT-1-WATER

Quant Time: Dec 16 04:06:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

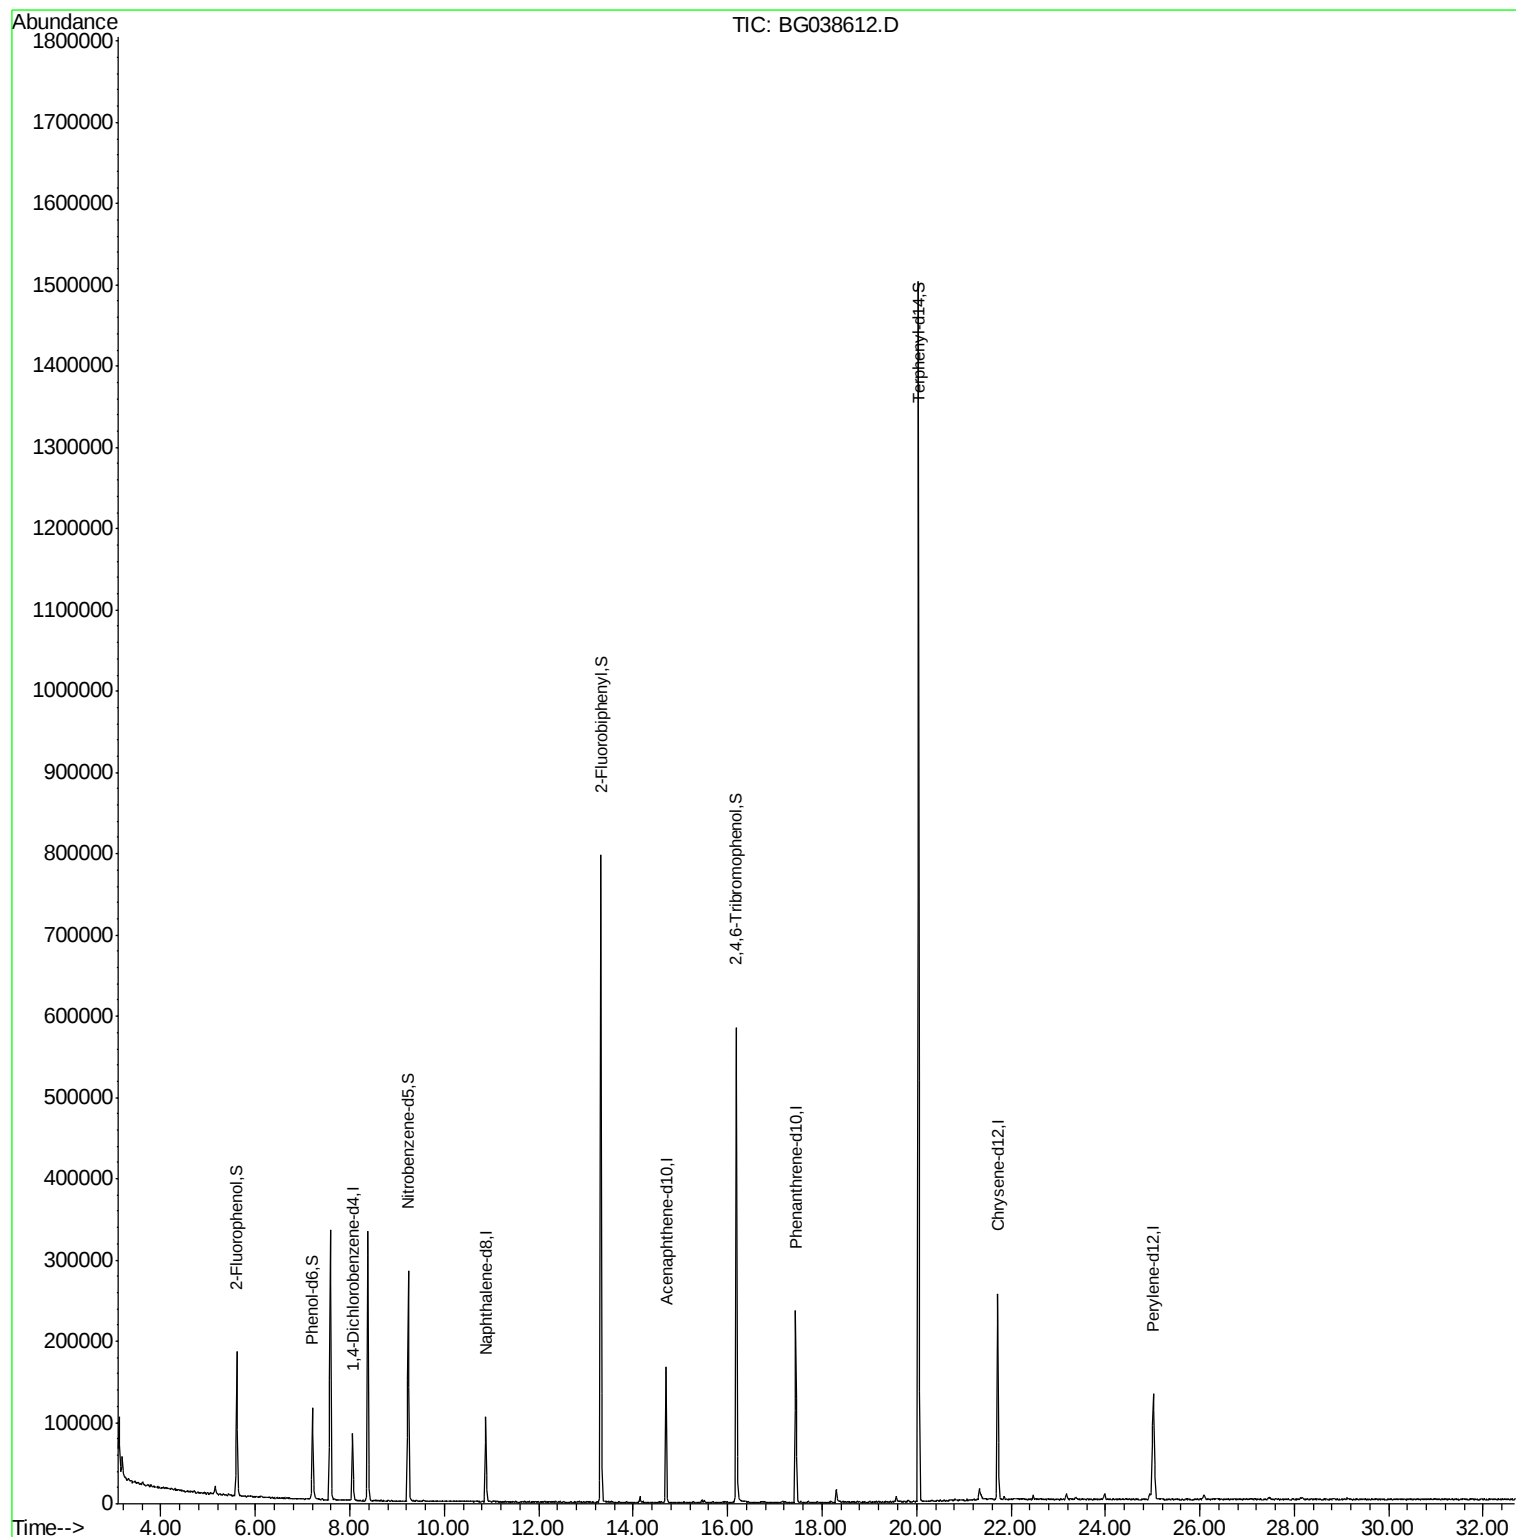




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.06 min Scan# 846
Delta R.T. -0.00 min
Lab File: BG038612.D
Acq: 15 Dec 2018 20:06

Instrument :
BNA_G
ClientSampleId :
TEST-PIT-1-WATER

Tot Ion:152 Resp: 23520
Ion Ratio Lower Upper
152 100
150 151.0 119.5 179.3
115 51.8 49.6 74.4

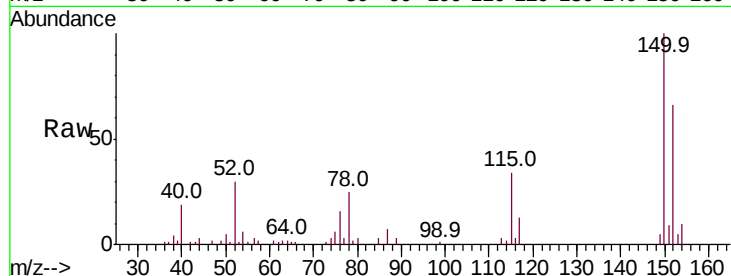


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

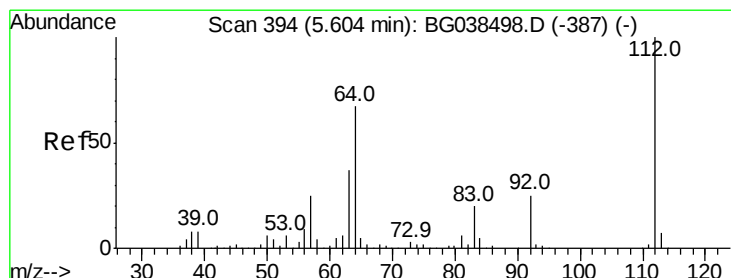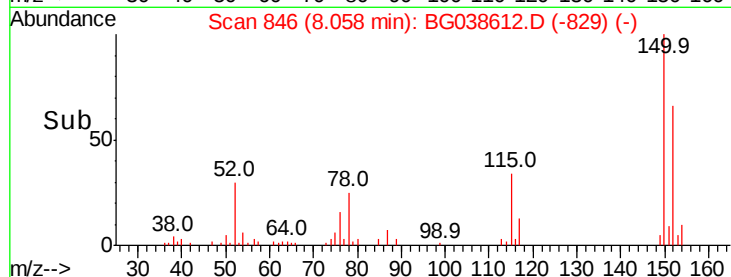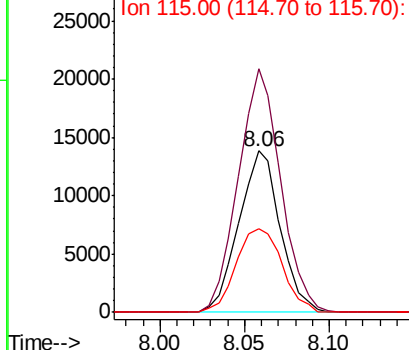



#5


2-Fluorophenol
Concen: 58.279 ng
RT: 5.61 min Scan# 429
Delta R.T. 0.01 min
Lab File: BG038612.D
Acq: 15 Dec 2018 20:06

Tgt Ion:112 Resp: 77282
Ion Ratio Lower Upper
112 100
64 64.8 53.4 80.2
63 38.0 29.3 43.9

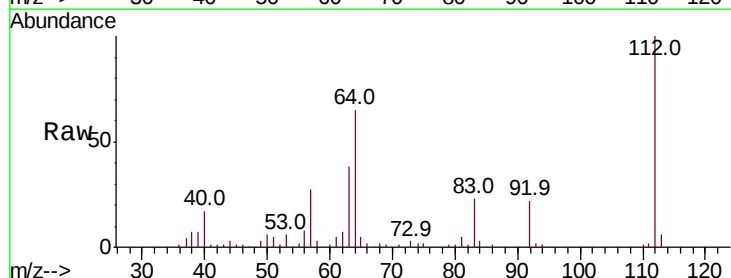

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

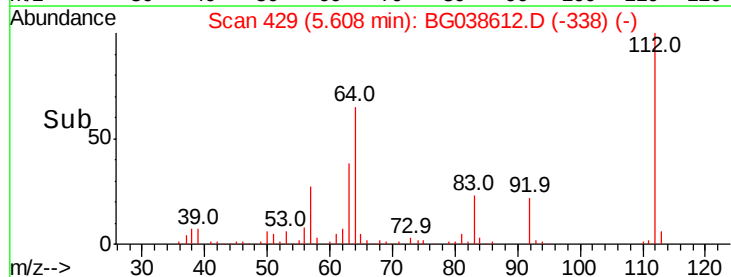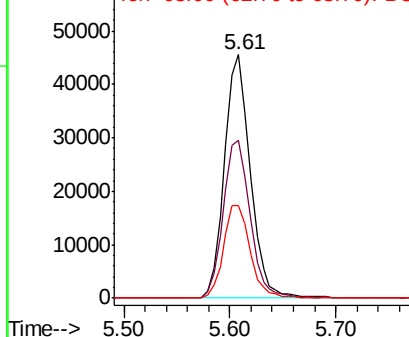

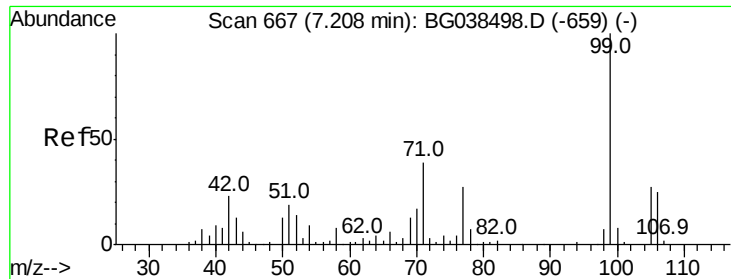

#7

Phenol-d6

Concen: 34.927 ng

RT: 7.21 min Scan# 701

Delta R.T. -0.00 min

Lab File: BG038612.D

Acq: 15 Dec 2018 20:06

Instrument :

BNA_G

ClientSampleId :

TEST-PIT-1-WATER


Tot Ion: 99 Resp: 63583

Ion Ratio Lower Upper




99 100

42 25.8 18.5 27.7

71 40.8 31.1 46.7

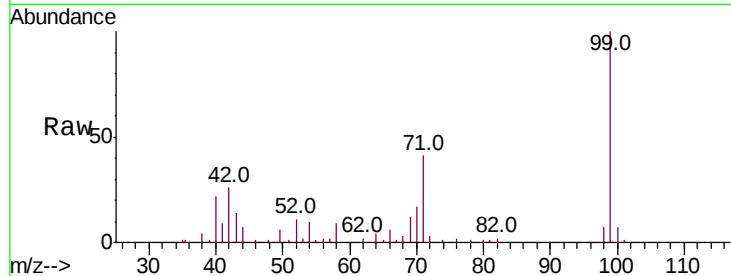

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

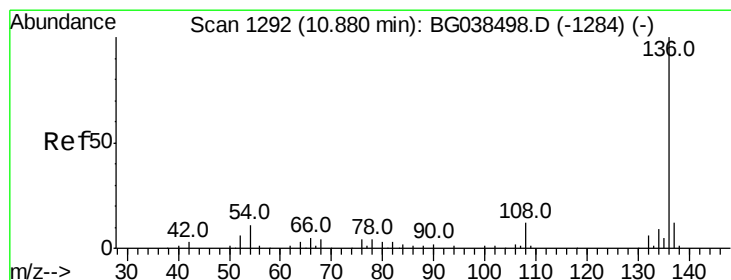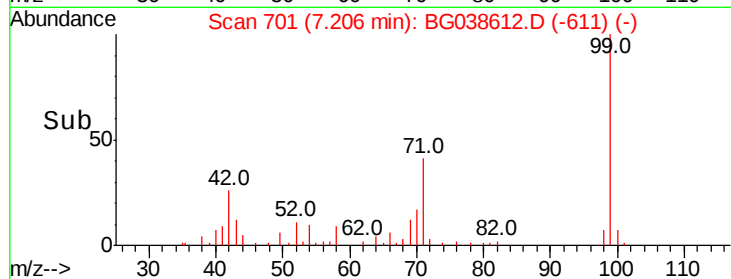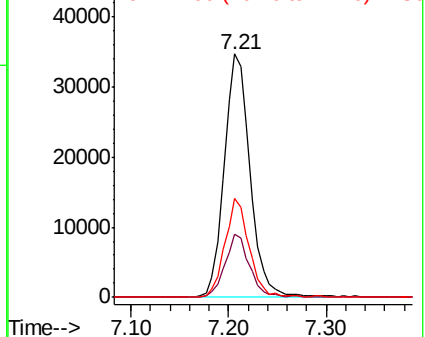

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.88 min Scan# 1326

Delta R.T. -0.00 min

Lab File: BG038612.D

Acq: 15 Dec 2018 20:06

Tgt Ion: 136 Resp: 94567


Ion Ratio Lower Upper

136 100



137 11.5 9.3 13.9

54 11.5 8.5 12.7

68 5.3 3.5 5.3#

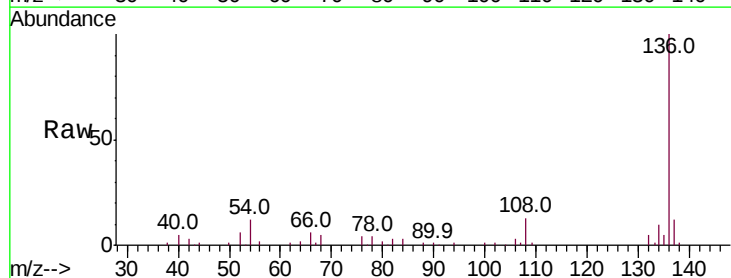

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC


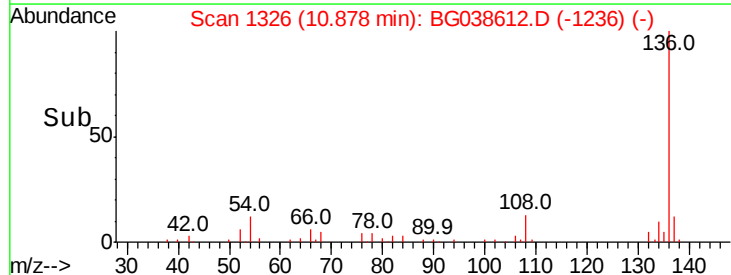
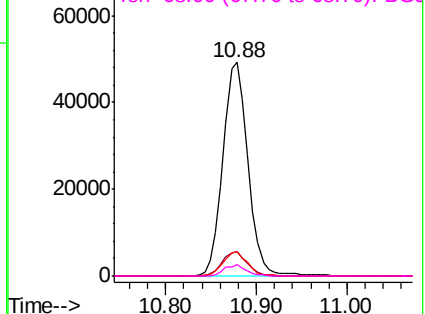




#23
 Nitrobenzene-d5
 Concen: 93.416 ng
 RT: 9.24 min Scan# 1047
 Delta R.T. -0.00 min
 Lab File: BG038612.D
 Acq: 15 Dec 2018 20:06




Instrument :
 BNA_G
 ClientSampleId :
 TEST-PIT-1-WATER

Tot Ion: 82 Resp: 172921
 Ion Ratio Lower Upper
 82 100
 128 44.5 34.6 52.0
 54 65.6 50.6 76.0

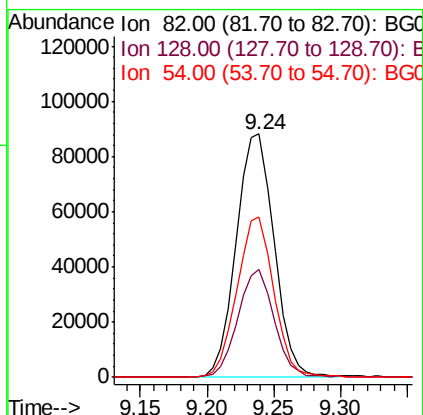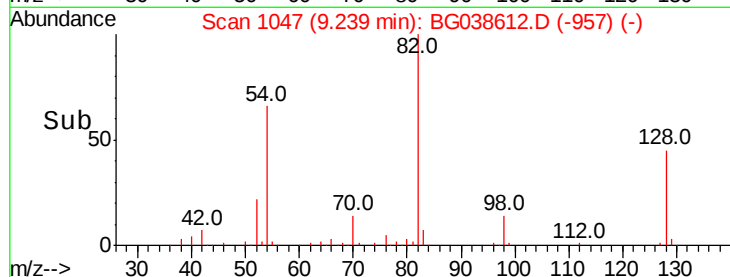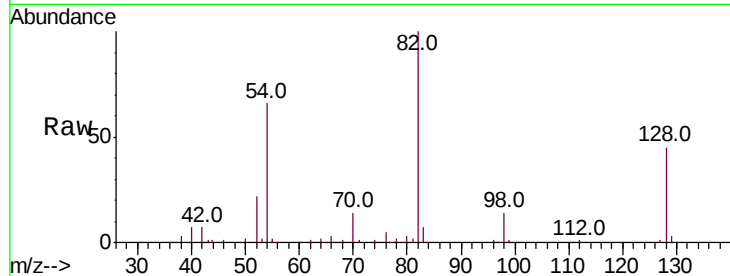

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.70 min Scan# 1976
 Delta R.T. -0.00 min
 Lab File: BG038612.D
 Acq: 15 Dec 2018 20:06

Tgt Ion:164 Resp: 60434
 Ion Ratio Lower Upper
 164 100
 162 105.2 86.6 130.0
 160 45.5 34.2 51.2

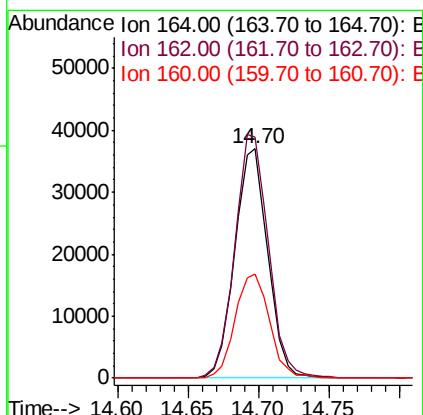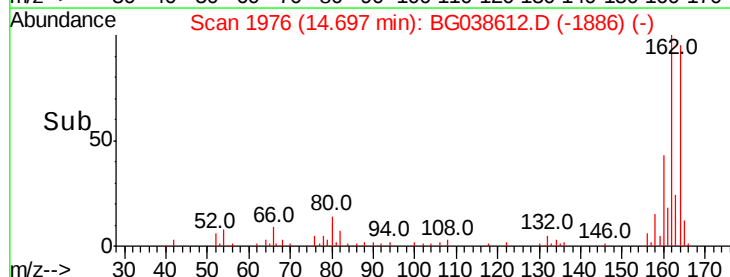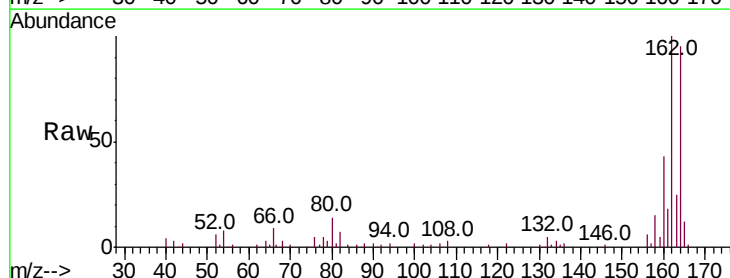







#42
 2,4,6-Tribromophenol
 Concen: 140.740 ng
 RT: 16.19 min Scan# 2230
 Delta R.T. -0.00 min
 Lab File: BG038612.D
 Acq: 15 Dec 2018 20:06

Instrument :
 BNA_G
 ClientSampleId :
 TEST-PIT-1-WATER

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.3	76.9	115.3
141	36.9	28.8	43.2

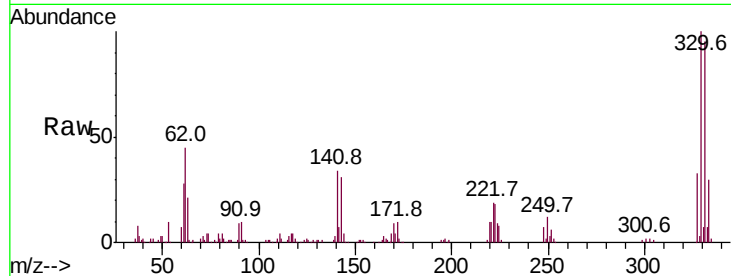


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

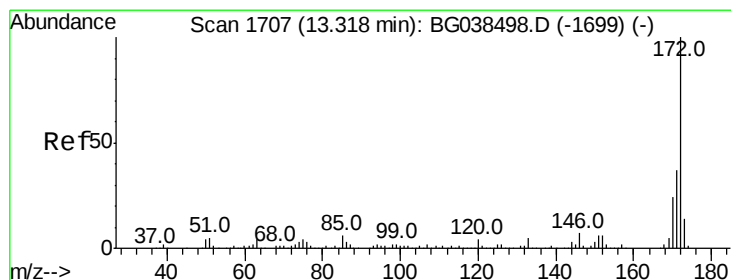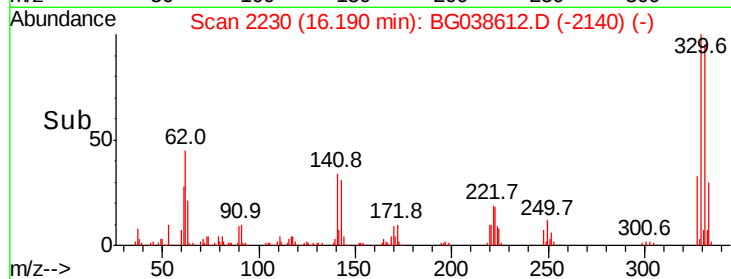
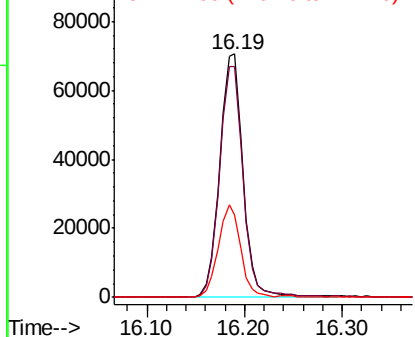



#45
 2-Fluorobiphenyl
 Concen: 94.021 ng
 RT: 13.32 min Scan# 1741
 Delta R.T. -0.00 min
 Lab File: BG038612.D
 Acq: 15 Dec 2018 20:06

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.0	29.8	44.6
170	24.7	19.5	29.3

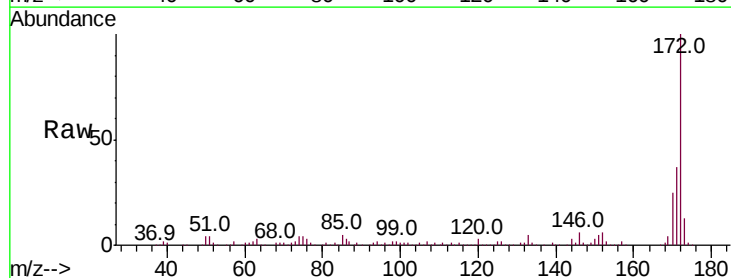

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

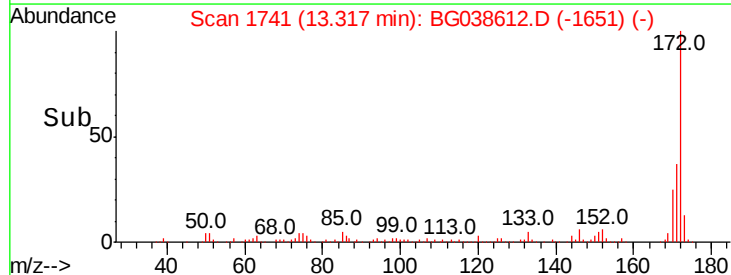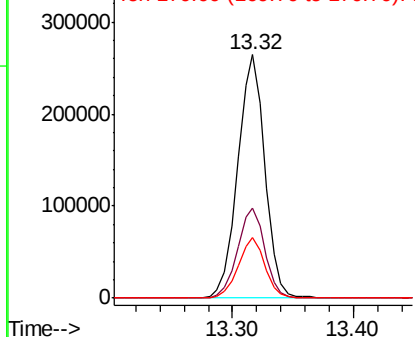


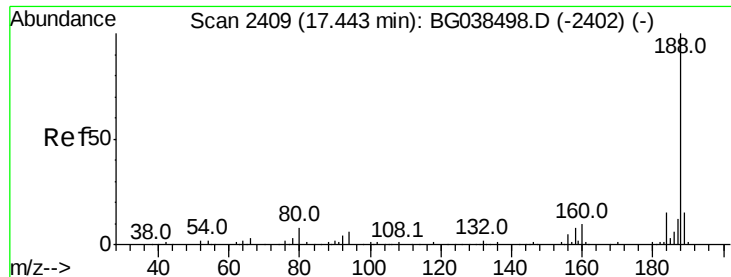




#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.44 min Scan# 2443
 Delta R.T. -0.00 min
 Lab File: BG038612.D
 Acq: 15 Dec 2018 20:06

Instrument :
 BNA_G
 ClientSampleId :
 TEST-PIT-1-WATER

Tot Ion:188 Resp: 151603
 Ion Ratio Lower Upper
 188 100
 94 6.7 5.1 7.7
 80 7.4 6.1 9.1

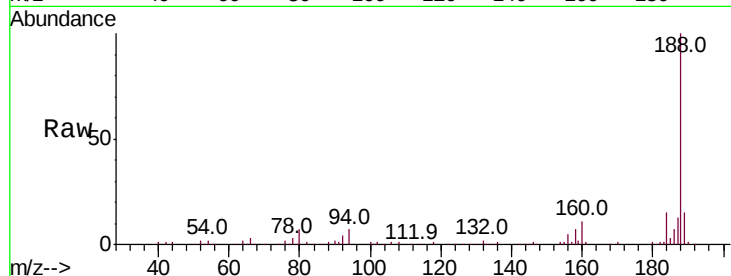


Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BG
 Ion 80.00 (79.70 to 80.70): BG

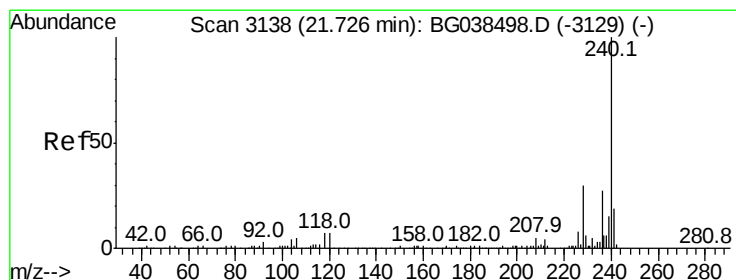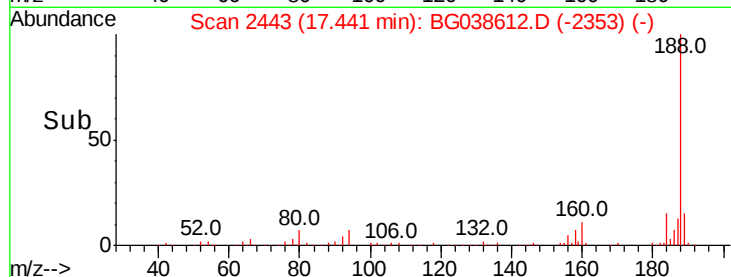
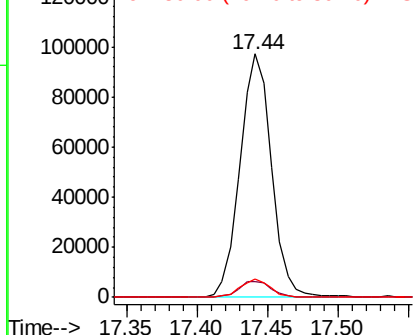


#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.72 min Scan# 3171
 Delta R.T. -0.01 min
 Lab File: BG038612.D
 Acq: 15 Dec 2018 20:06

Tgt Ion:240 Resp: 158143
 Ion Ratio Lower Upper
 240 100
 120 6.7 5.3 7.9
 236 25.4 21.4 32.2

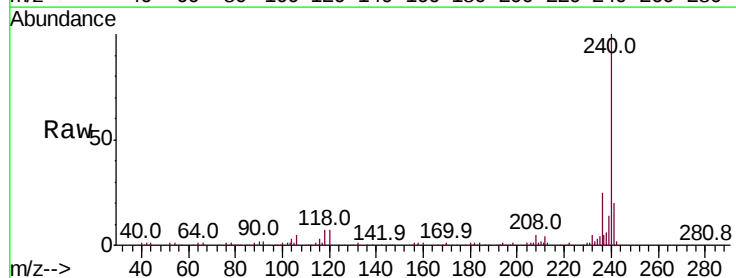

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

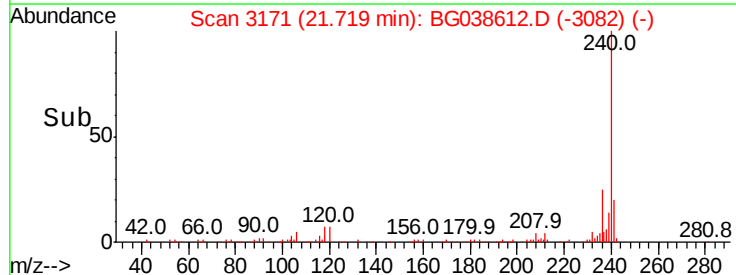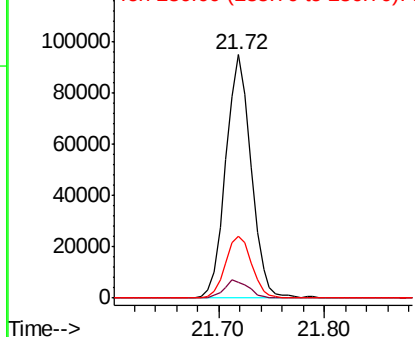



#79

Terphenyl-d14

Concen: 102.545 ng

RT: 20.04 min Scan# 2886

Delta R.T. -0.00 min

Lab File: BG038612.D

Acq: 15 Dec 2018 20:06

Instrument :

BNA_G

ClientSampleId :

TEST-PIT-1-WATER


Tot Ion:244 Resp: 745139

Ion Ratio Lower Upper

244 100

212 8.0 6.2 9.2




122 7.0 6.3 9.5

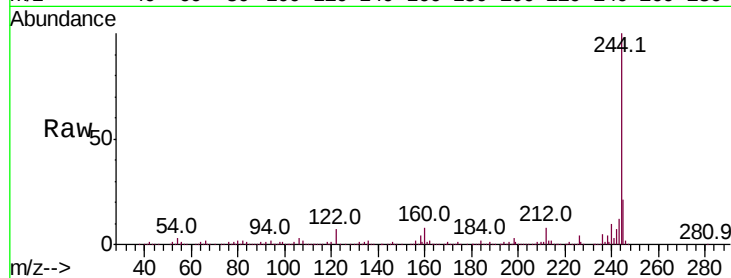

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

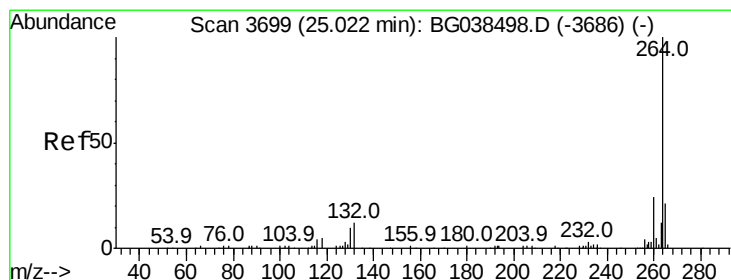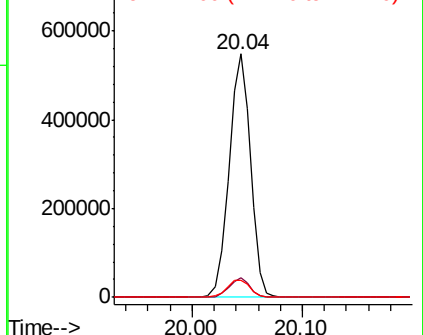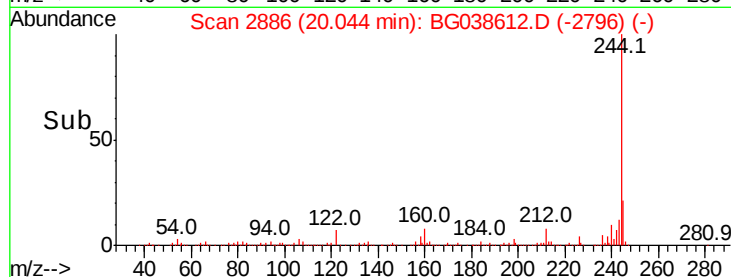

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.01 min Scan# 3732

Delta R.T. -0.01 min

Lab File: BG038612.D

Acq: 15 Dec 2018 20:06


Tgt Ion:264 Resp: 166019

Ion Ratio Lower Upper

264 100

260 23.5 18.9 28.3

265 21.2 17.0 25.4

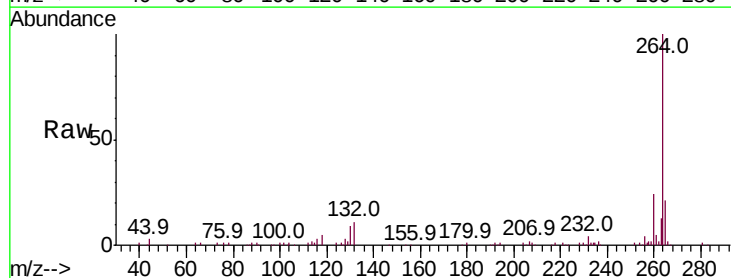

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

