

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG121518\
 Data File : BG038612.D
 Acq On : 15 Dec 2018 20:06
 Operator : JU/SJ
 Sample : J6376-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TEST-PIT-1-WATER

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.182	13	16	27	rVB2	28256	50521	2.49%	0.603%
2	5.608	422	429	439	rBV	178110	307043	15.14%	3.664%
3	7.206	695	701	713	rBV	112488	208331	10.27%	2.486%
4	7.588	757	766	776	rBV	333370	609995	30.07%	7.279%
5	8.058	840	846	853	rVB	82935	140756	6.94%	1.680%
6	8.381	893	901	909	rVB	330829	594693	29.32%	7.096%
7	9.239	1039	1047	1058	rBV	283251	543248	26.78%	6.483%
8	10.878	1318	1326	1335	rBV	104376	197210	9.72%	2.353%
9	13.317	1733	1741	1751	rBV	796248	1244584	61.35%	14.851%
10	14.697	1969	1976	1986	rVB2	167140	282590	13.93%	3.372%
11	16.184	2222	2229	2240	rBV2	584515	933062	46.00%	11.134%
12	17.441	2437	2443	2452	rBV2	235469	361766	17.83%	4.317%
13	18.299	2585	2589	2597	rBV3	15940	26551	1.31%	0.317%
14	20.044	2880	2886	2898	rBV	1501414	2028528	100.00%	24.206%
15	21.325	3099	3104	3116	rBV8	13862	38175	1.88%	0.456%
16	21.719	3163	3171	3178	rBV2	253877	422817	20.84%	5.045%
17	25.015	3722	3732	3744	rVB	129442	390349	19.24%	4.658%


Sum of corrected areas: 8380219

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG121518\
Data File : BG038612.D
Acq On : 15 Dec 2018 20:06
Operator : JU/SJ
Sample : J6376-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TEST-PIT-1-WATER

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

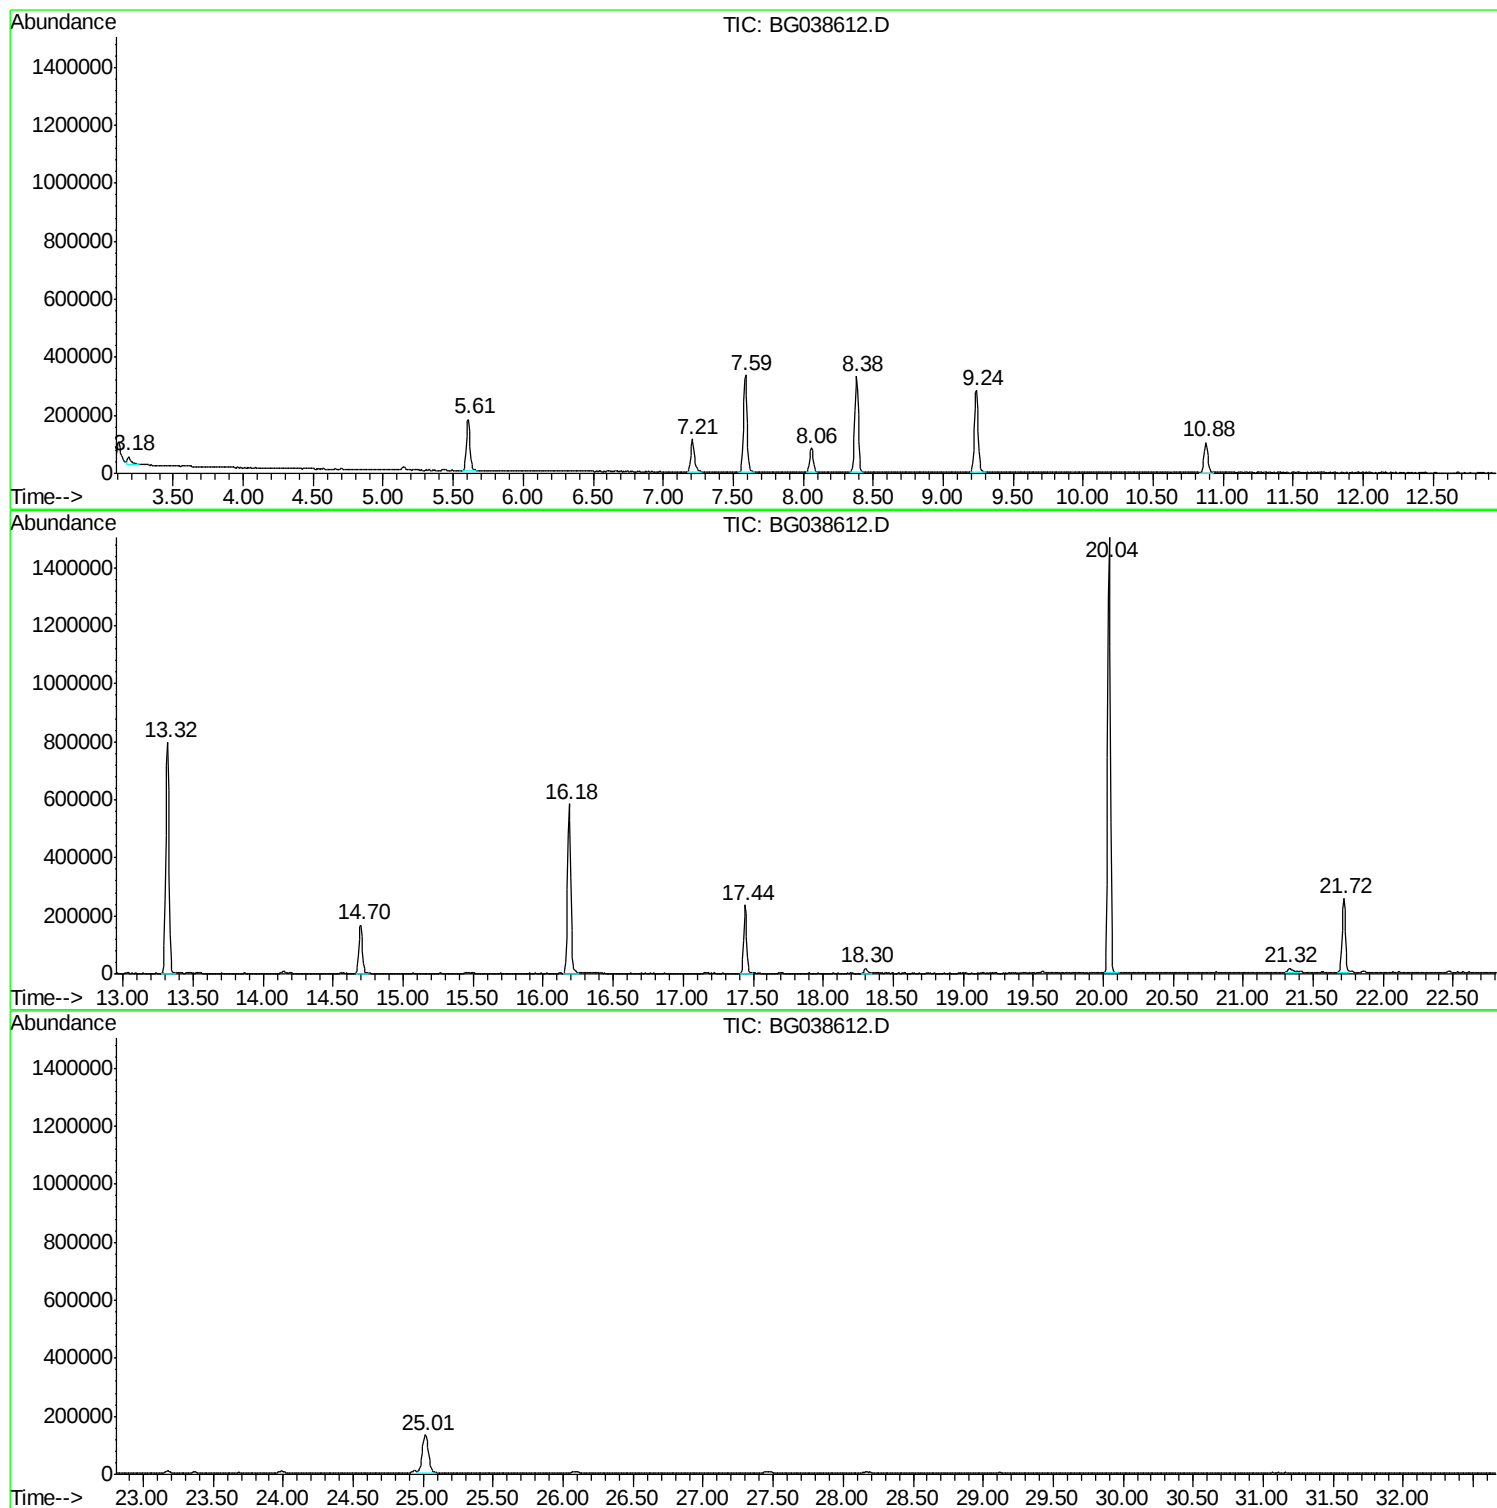

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG121518\
Data File : BG038612.D
Acq On : 15 Dec 2018 20:06
Operator : JU/SJ
Sample : J6376-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TEST-PIT-1-WATER










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.18	7.18 ng	50521	1,4-Dichlorobenzene-d4	8.06

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64
2		3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	28
3		2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	23
4		3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	23
5		Acetamide, N-(2-hydroxy-3-penten...	143	C7H13NO2	093393-95-4	9

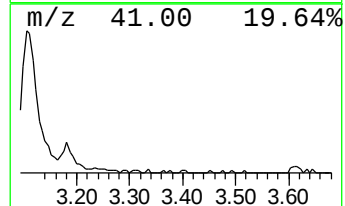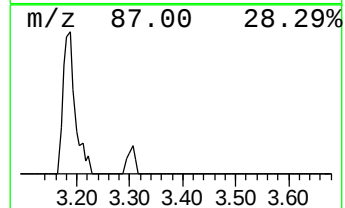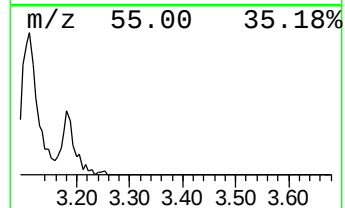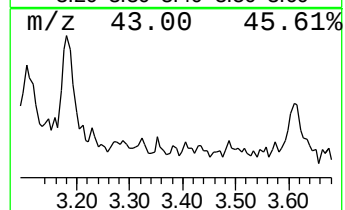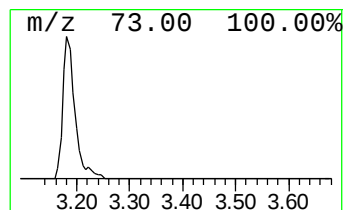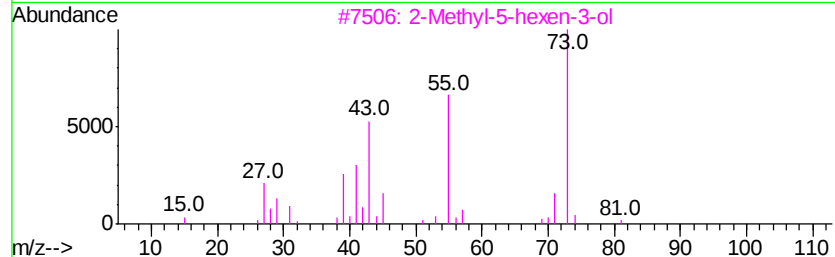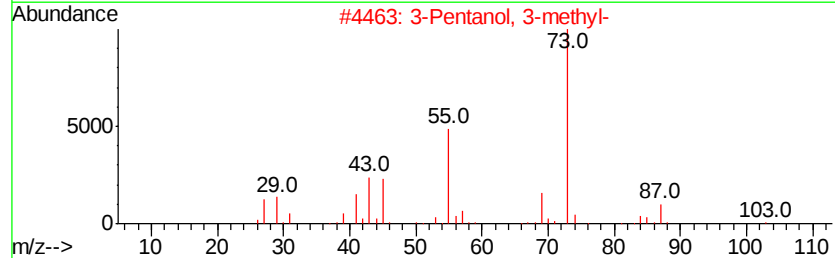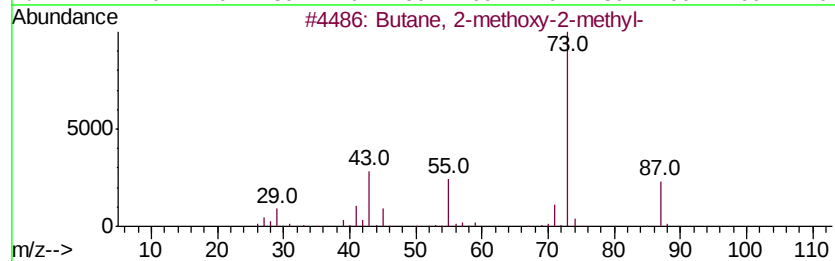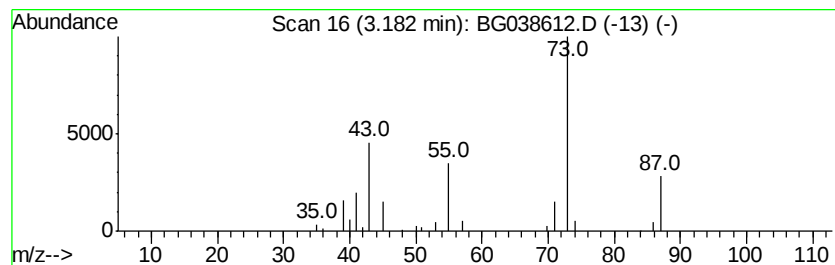

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG121518\
Data File : BG038612.D
Acq On : 15 Dec 2018 20:06
Operator : JU/SJ
Sample : J6376-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TEST-PIT-1-WATER










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.59 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.59	86.67 ng	609995	1,4-Dichlorobenzene-d4	8.06

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
3		Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
5		Pyrazolo(2,3-a)pyridine, 7-methyl-	132	C8H8N2	034760-58-2	12

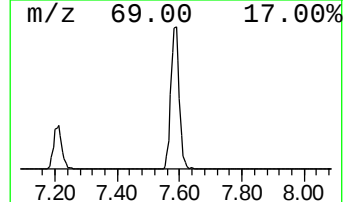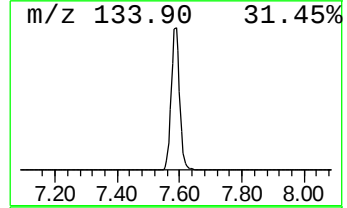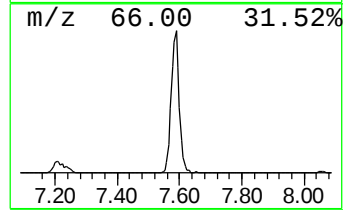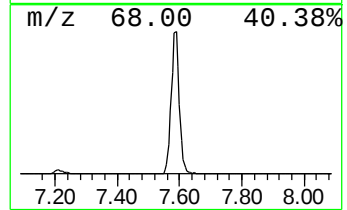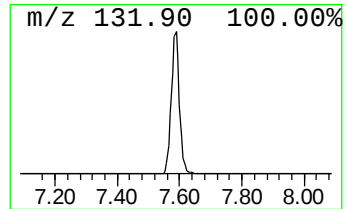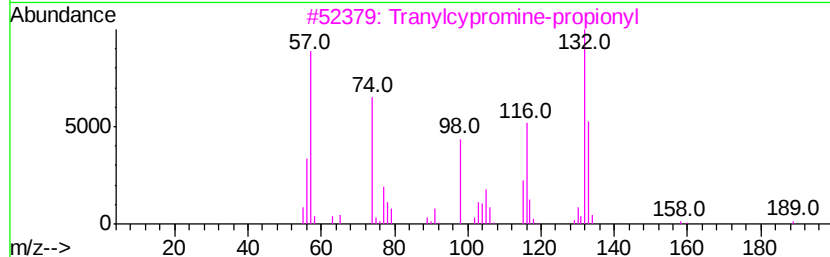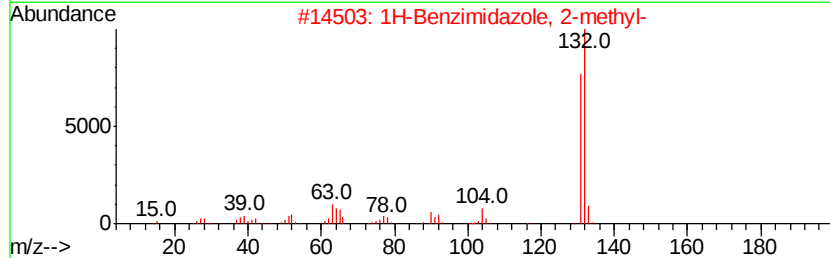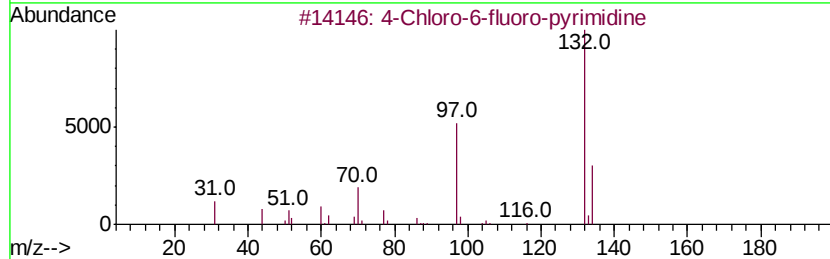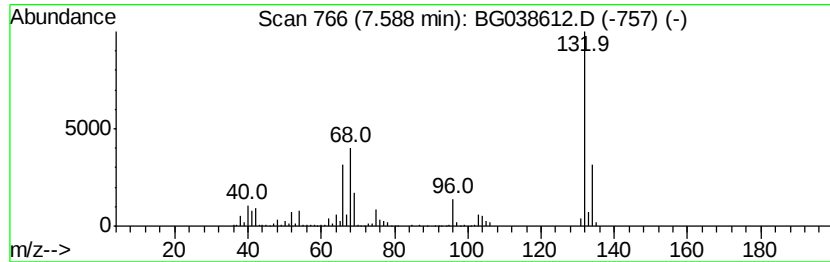

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG121518\
Data File : BG038612.D
Acq On : 15 Dec 2018 20:06
Operator : JU/SJ
Sample : J6376-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TEST-PIT-1-WATER

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	3.18	7.2	ng	50521	1	8.06	140756	20.0
unknown7.59	7.59	86.7	ng	609995	1	8.06	140756	20.0