


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121518\
 Data File : BG038599.D
 Acq On : 15 Dec 2018 11:34
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

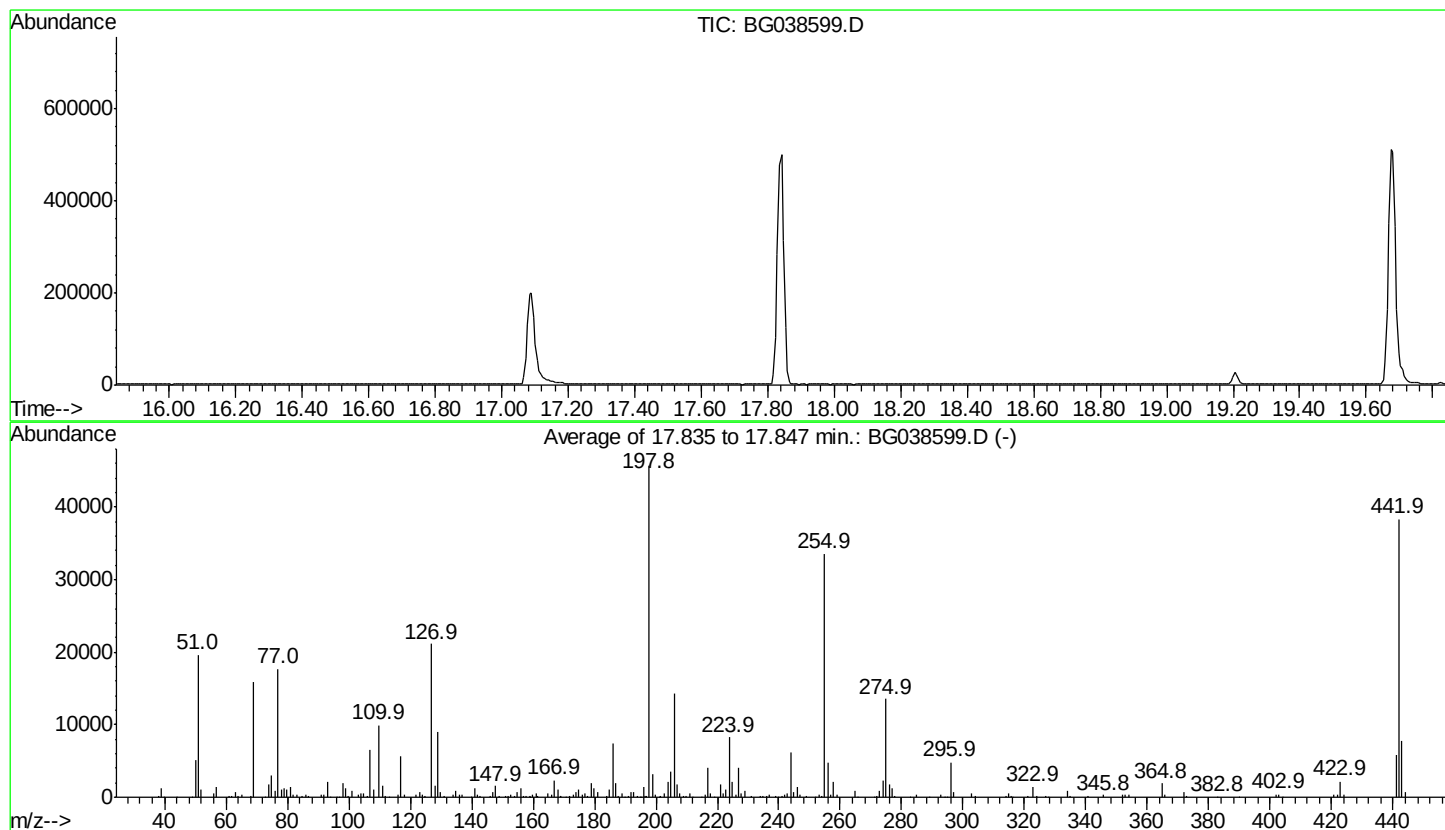

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.9	19606	PASS
68	69	0.00	2	1.2	190	PASS
69	198	0.00	100	34.8	15900	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.2	21116	PASS
197	198	0.00	2	0.2	109	PASS
198	198	100	100	100.0	45733	PASS
199	198	5	9	7.0	3200	PASS
275	198	10	60	29.6	13556	PASS
365	198	1	100	4.2	1921	PASS
441	198	0.01	100	12.7	5820	PASS
442	198	50	100	83.8	38346	PASS
443	442	15	24	20.4	7841	PASS