


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121518\
 Data File : BG038618.D
 Acq On : 16 Dec 2018 00:06
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

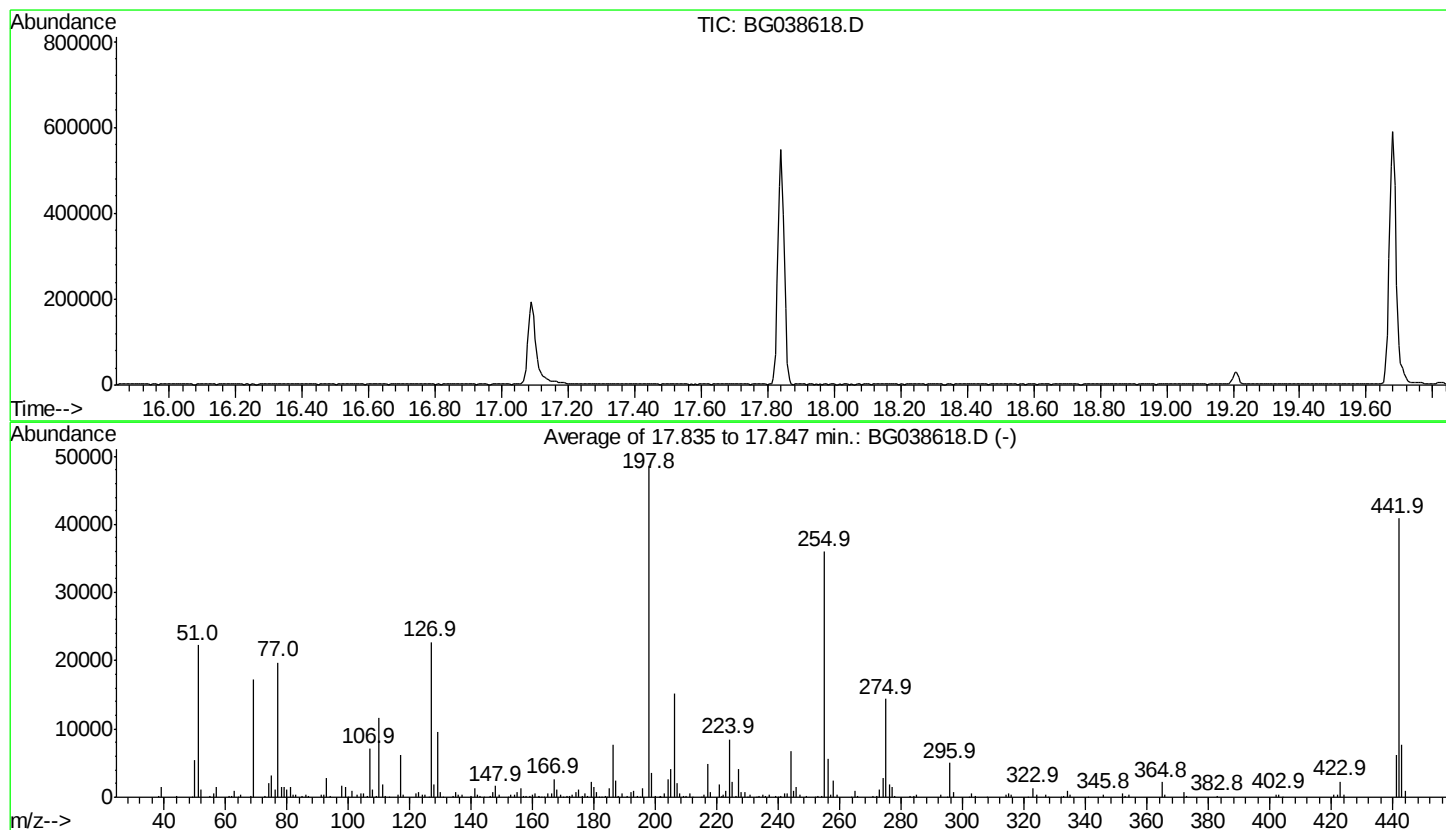

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.8	22265	PASS
68	69	0.00	2	1.0	166	PASS
69	198	0.00	100	35.6	17299	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.7	22712	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48602	PASS
199	198	5	9	7.3	3571	PASS
275	198	10	60	29.7	14424	PASS
365	198	1	100	4.5	2183	PASS
441	198	0.01	100	12.9	6251	PASS
442	198	50	100	84.1	40885	PASS
443	442	15	24	19.1	7789	PASS