


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121522\
 Data File : BG055973.D
 Acq On : 15 Dec 2022 12:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 14 02:24:06 2022

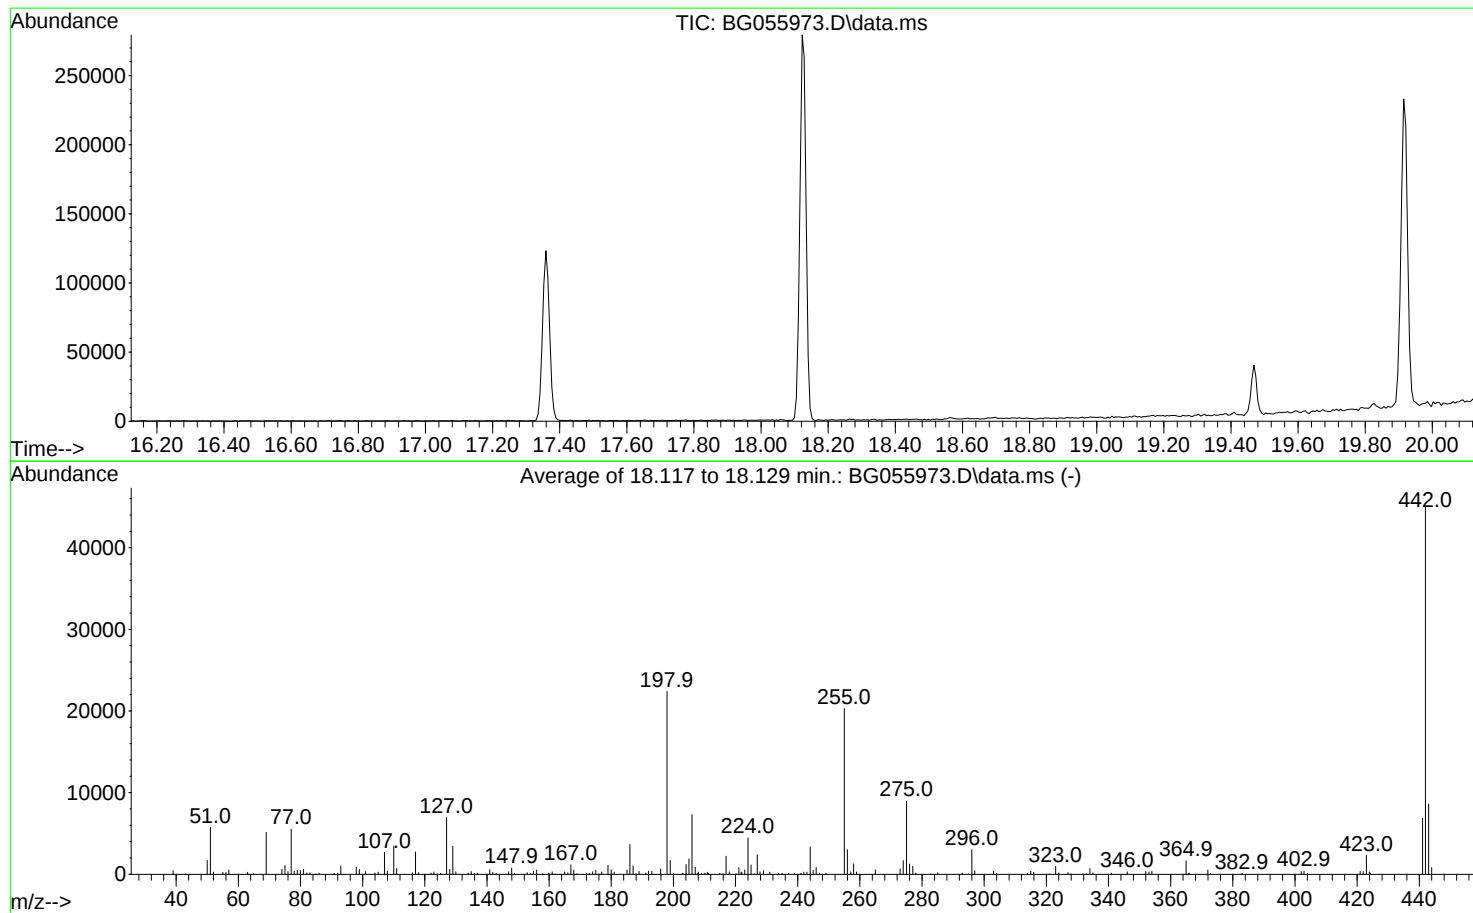




AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.7	5747	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	23.0	5145	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	31.0	6950	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22392	PASS
199	198	5	9	7.5	1671	PASS
275	198	10	60	40.0	8952	PASS
365	198	1	100	7.4	1657	PASS
441	198	0.01	100	30.6	6851	PASS
442	442	50	100	100.0	45056	PASS
443	442	15	24	19.1	8588	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121522\
Data File : BG055973.D
Acq On : 15 Dec 2022 12:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 16 07:34:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 14 02:24:06 2022
Response via : Initial Calibration

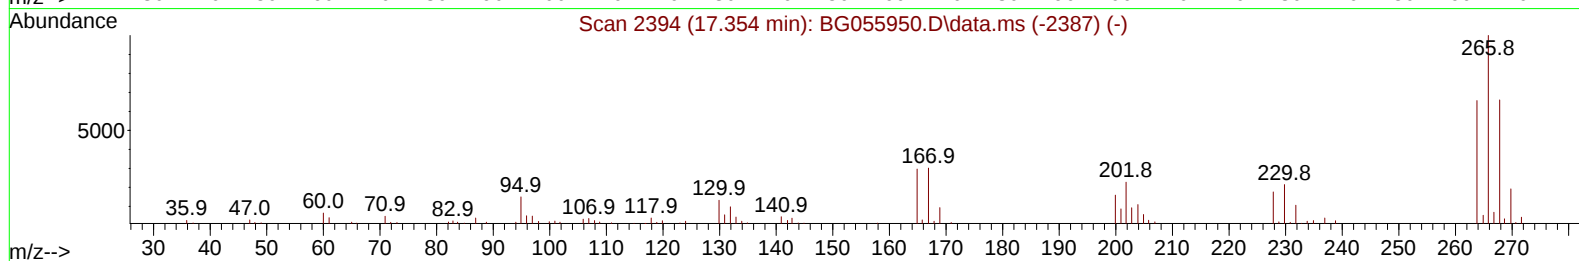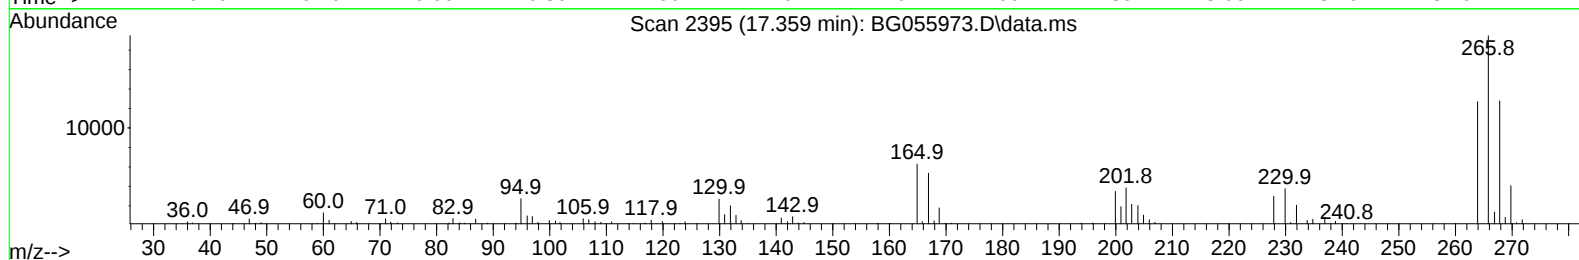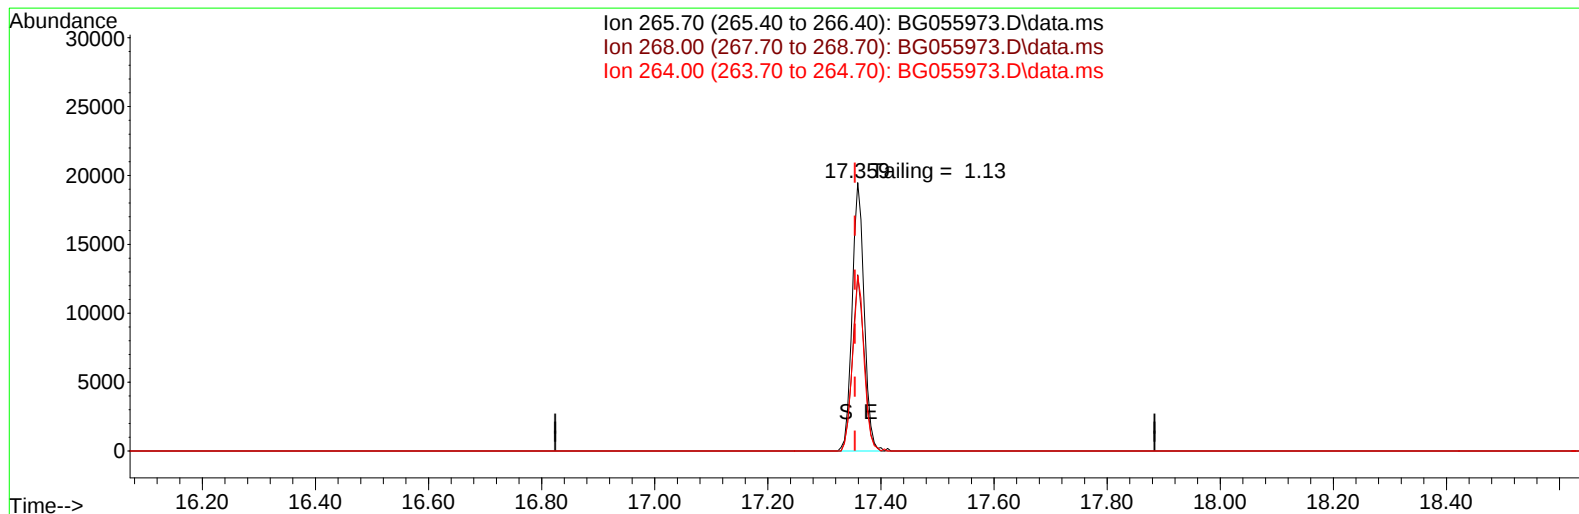

TIC: BG055973.D\data.ms

(70) Pentachlorophenol (C)

17.359min (+ 0.005) 37704.81 ng




response 28790

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.40	65.67
264.00	65.70	65.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121522\
Data File : BG055973.D
Acq On : 15 Dec 2022 12:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 16 07:34:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 14 02:24:06 2022
Response via : Initial Calibration

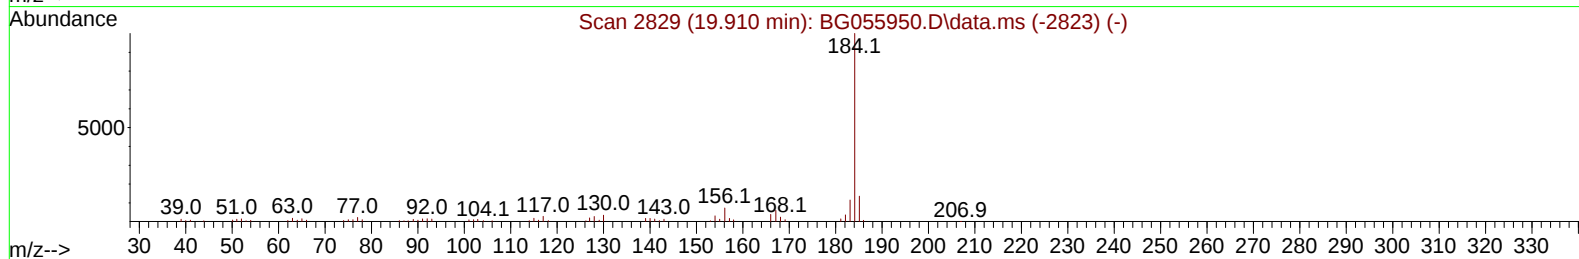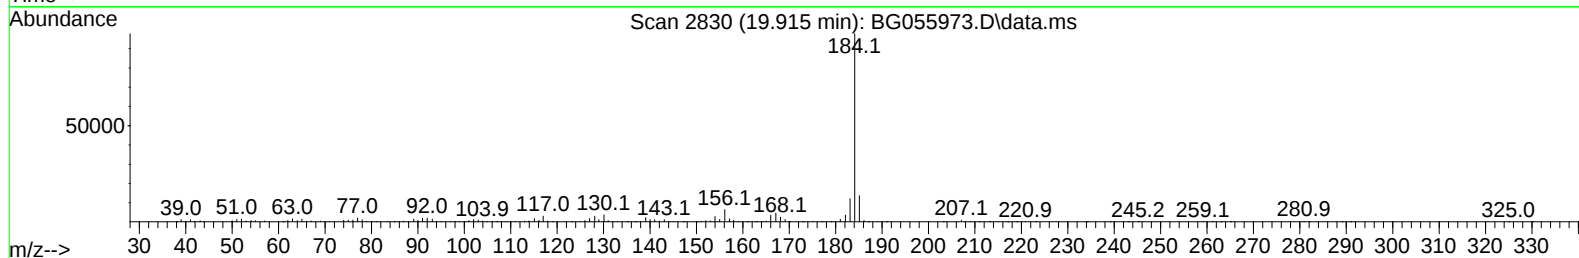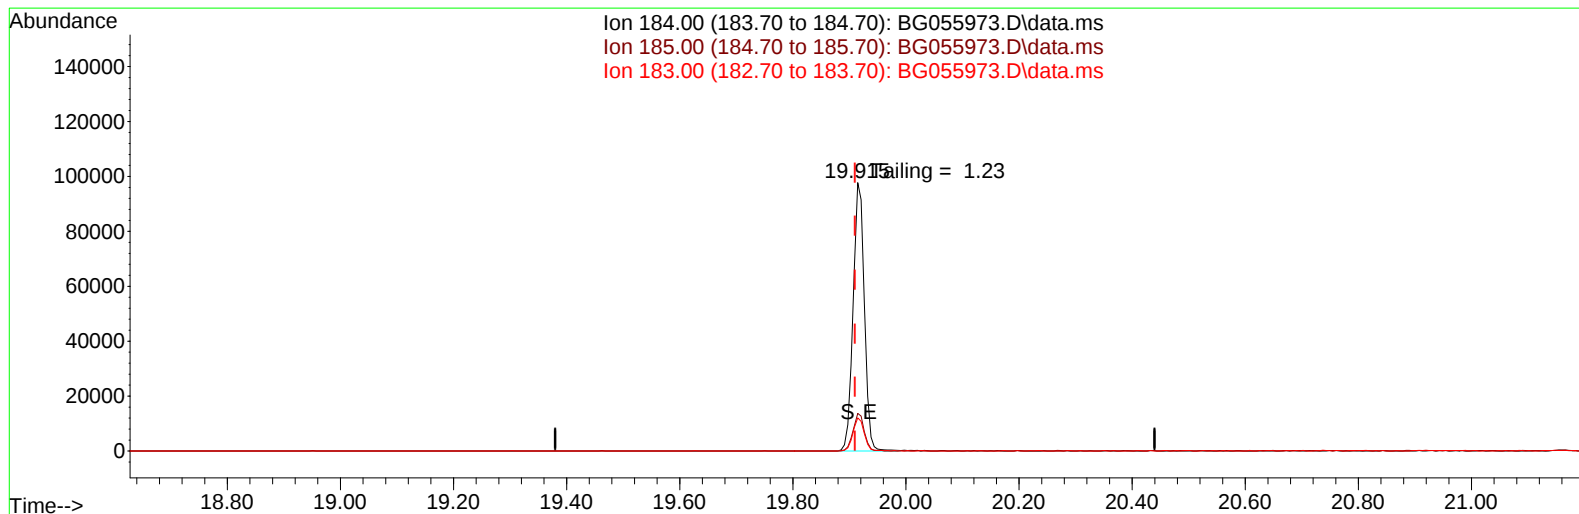

TIC: BG055973.D\data.ms

(77) Benzidine

19.915min (+ 0.005) 66386.67 ng

response 135240

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.00
183.00	11.50	12.38
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/15/2022	BNA_G	<u>BG055973.D</u>
Compound Name	Response	Retention Time
DDT	67146	21.16
DDD	2522	20.696
DDE	0	20.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2522	69668	3.62

Instrument :
BNA_G
ClientSampleId :
DFTPP