
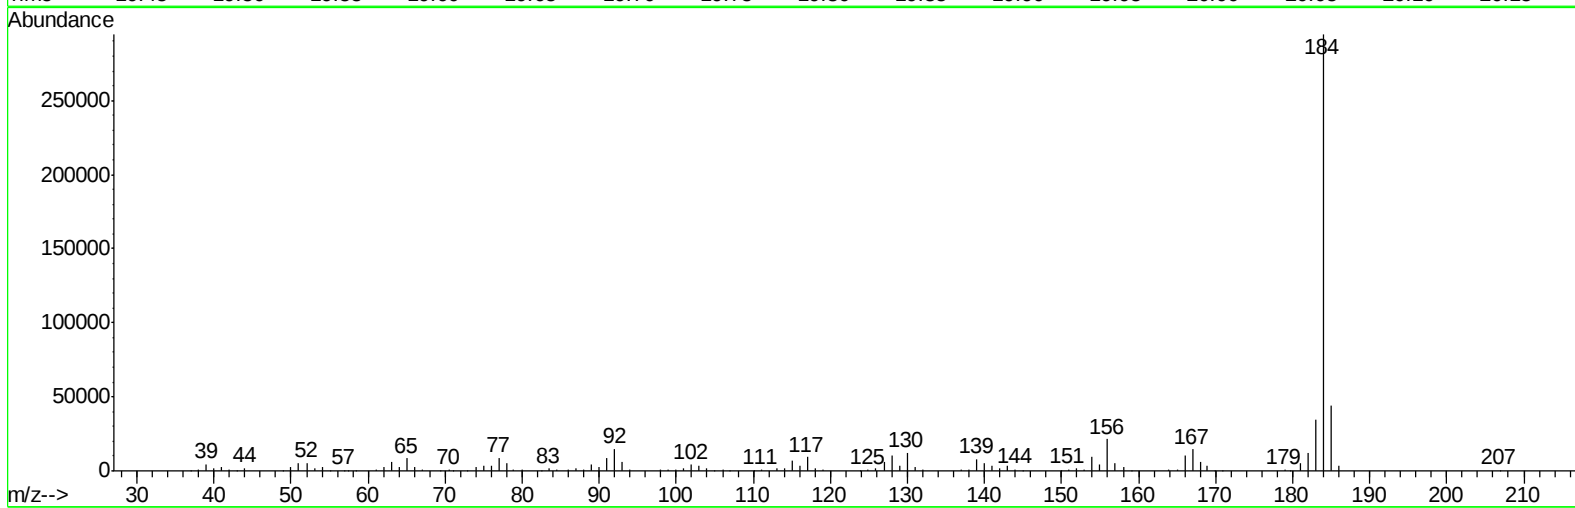


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG121618\
Data File : BG038635.D
Acq On : 16 Dec 2018 11:26
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 06:49:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

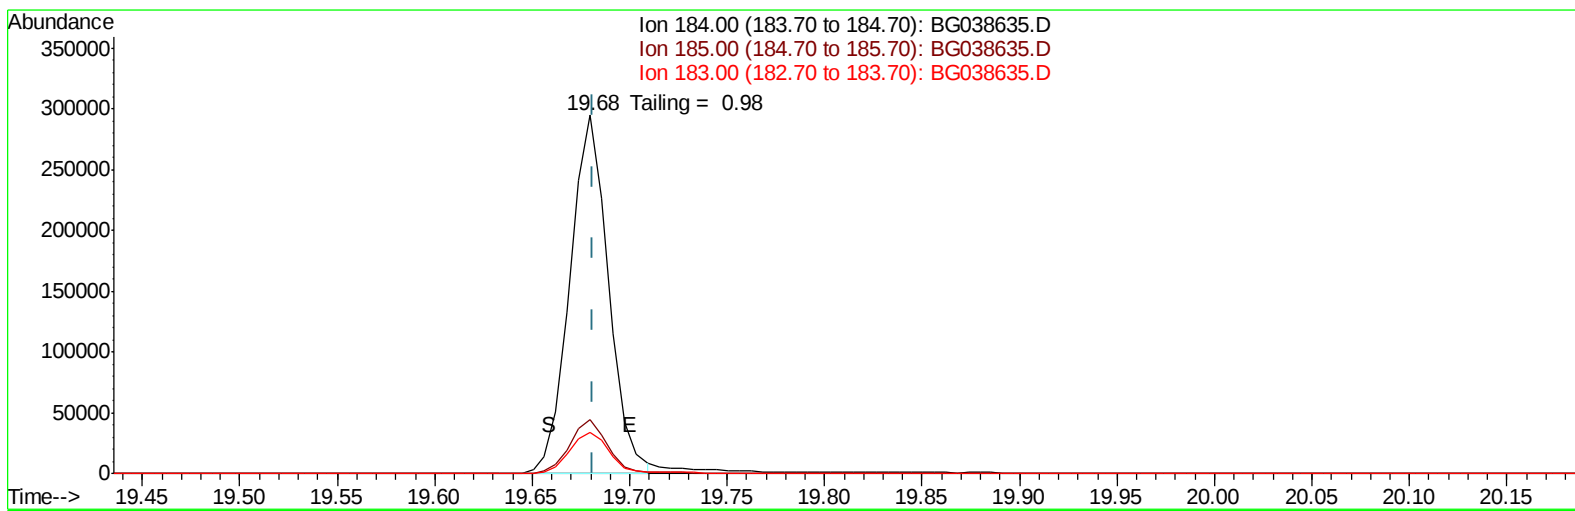

TIC: BG038635.D

(77) Benzidine



19.680min (-0.001) 266253.77ng

response 417333

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.02
183.00	12.00	11.61
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG121618\
Data File : BG038635.D
Acq On : 16 Dec 2018 11:26
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 06:49:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

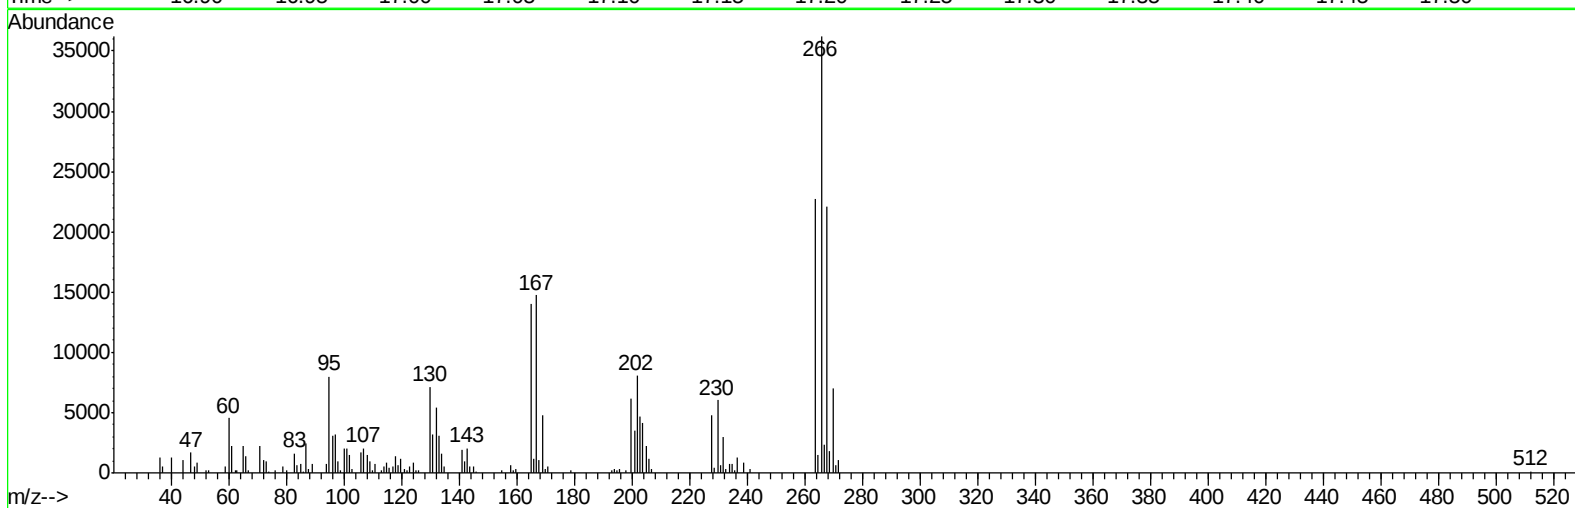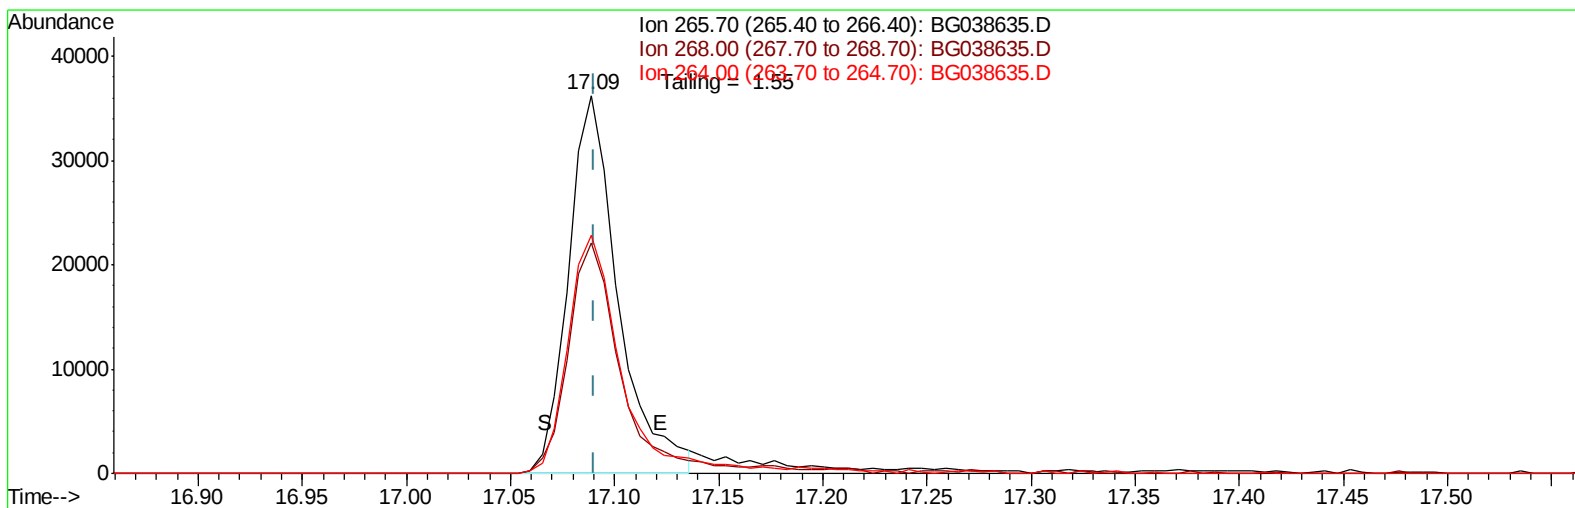

TIC: BG038635.D

(70) Pentachlorophenol (C)

17.089min (-0.001) 27978.31ng

response 64738

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	65.90
264.00	70.90	67.13
0.00	0.00	0.00