


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG121618\
 Data File : BG038635.D
 Acq On : 16 Dec 2018 11:26
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

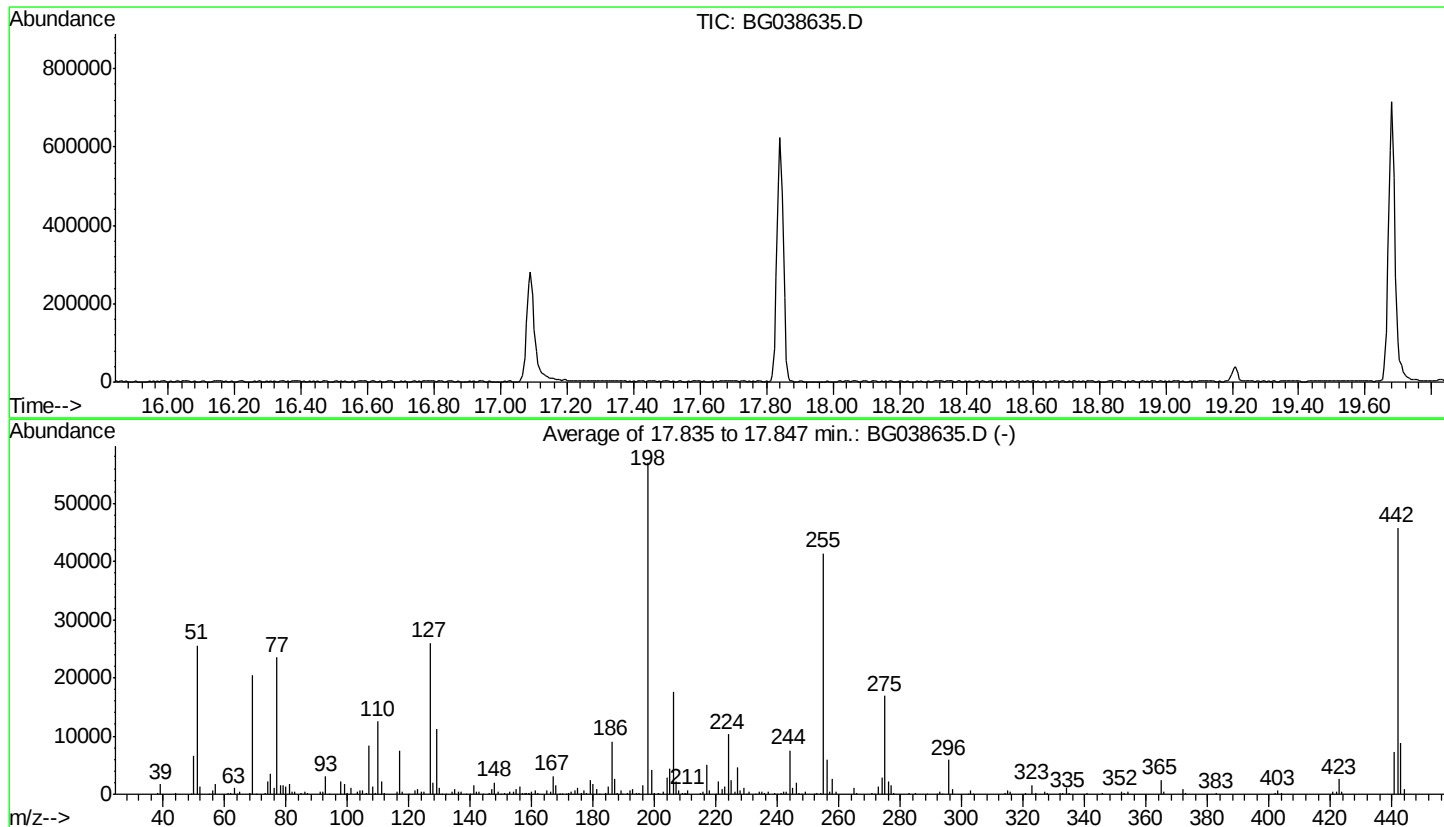

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.8	25546	PASS
68	69	0.00	2	0.8	167	PASS
69	198	0.00	100	35.9	20455	PASS
70	69	0.00	2	0.6	113	PASS
127	198	10	80	45.7	26061	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	57000	PASS
199	198	5	9	7.3	4146	PASS
275	198	10	60	29.6	16876	PASS
365	198	1	100	4.3	2479	PASS
441	198	0.01	100	12.6	7170	PASS
442	198	50	100	80.4	45840	PASS
443	442	15	24	19.0	8721	PASS