
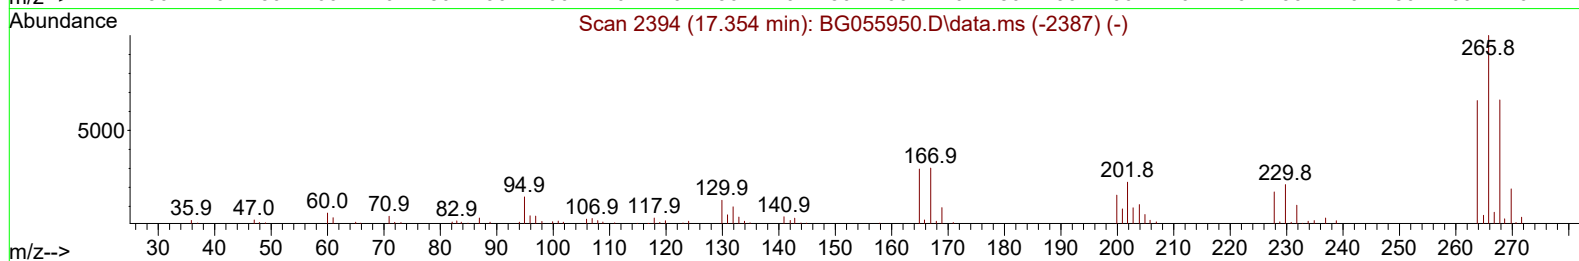
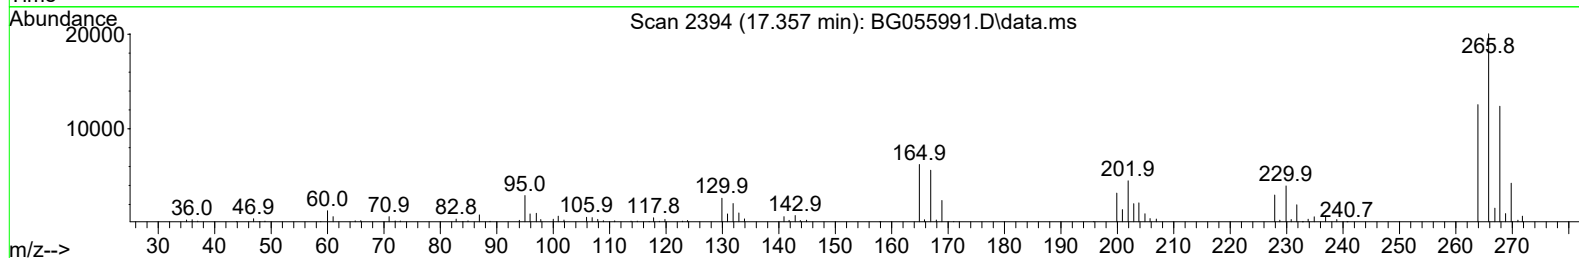


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121622\
Data File : BG055991.D
Acq On : 16 Dec 2022 12:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 06:16:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 01:18:54 2022
Response via : Initial Calibration

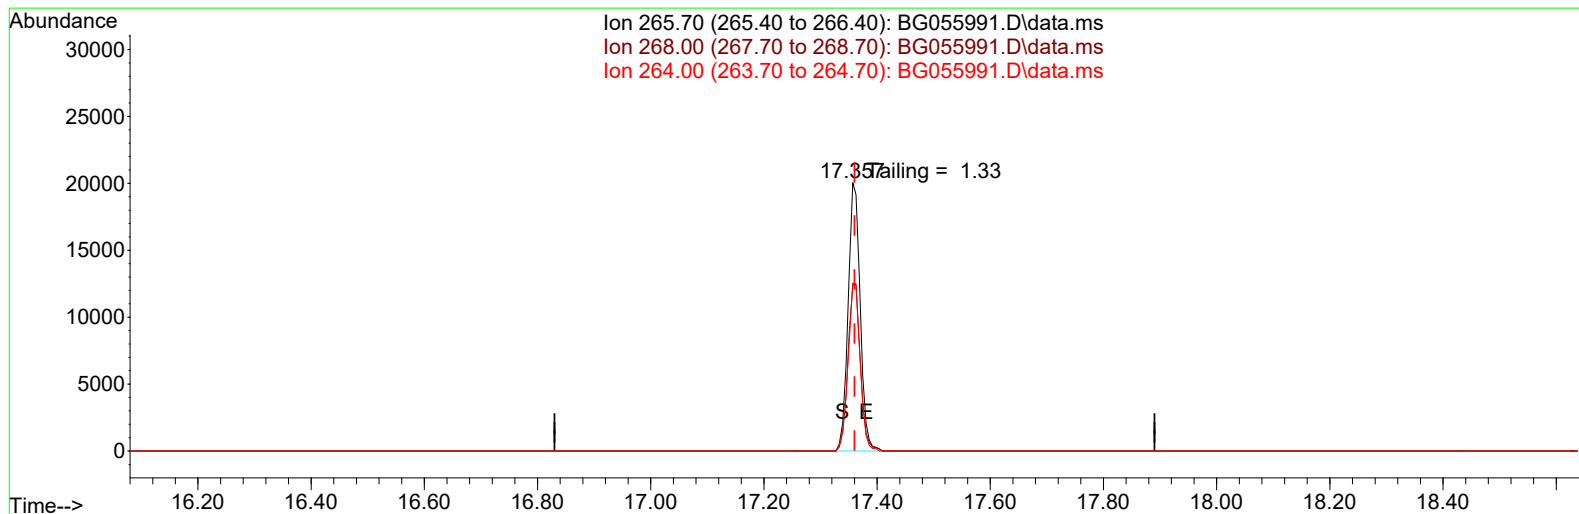

TIC: BG055991.D\data.ms

(70) Pentachlorophenol (C)




17.357min (-0.003) 6069.53 ng

response 29623

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.40	61.81
264.00	65.70	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121622\
Data File : BG055991.D
Acq On : 16 Dec 2022 12:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 06:16:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 01:18:54 2022
Response via : Initial Calibration

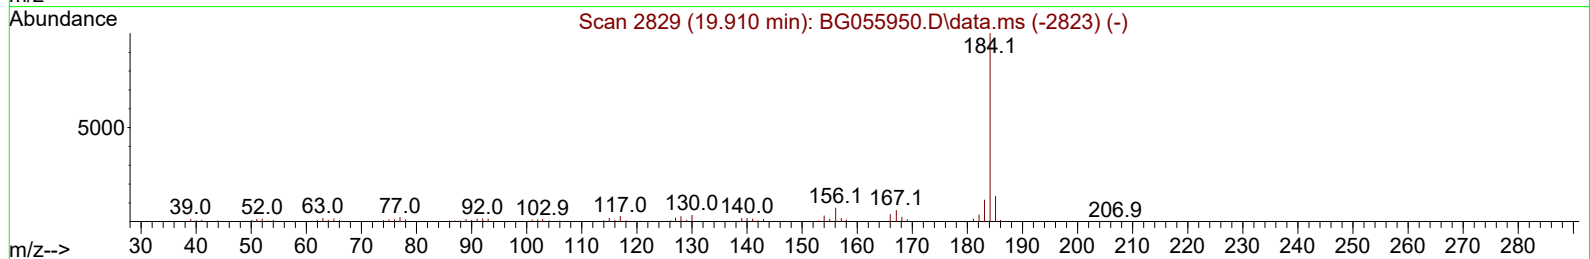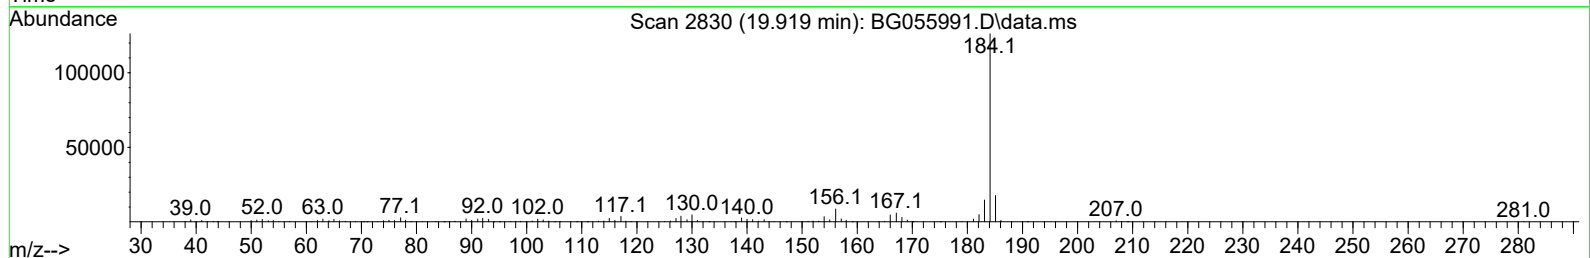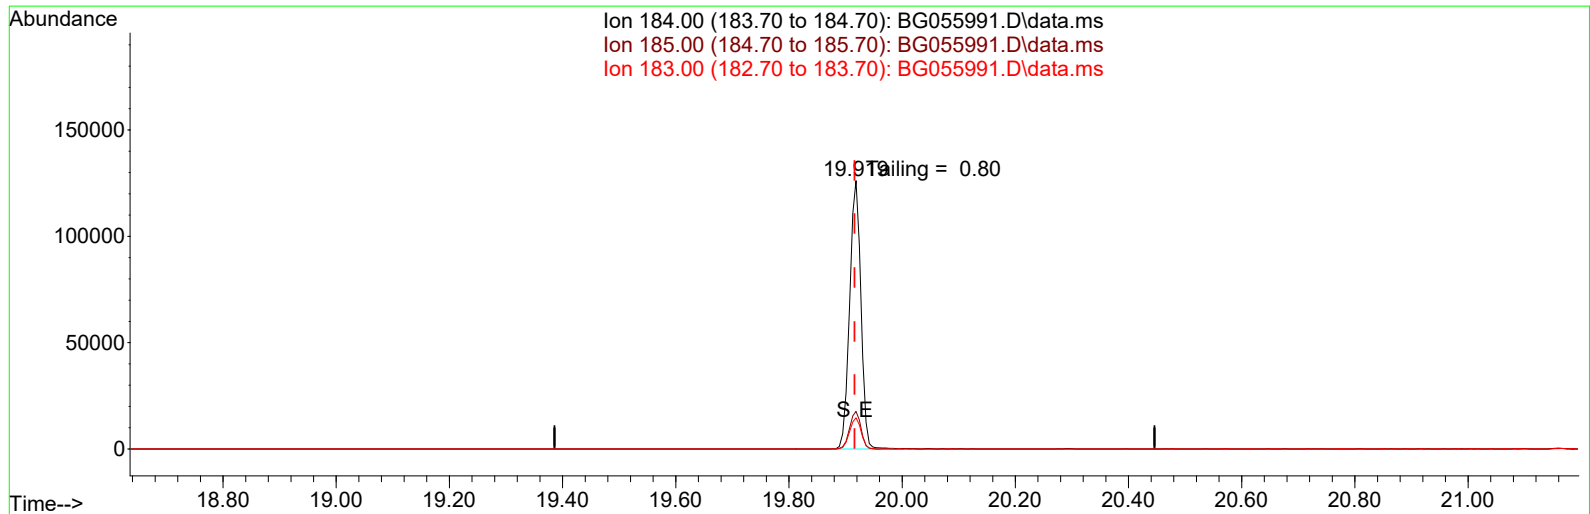

TIC: BG055991.D\data.ms

(77) Benzidine**19.919min (+ 0.003) 13015.78 ng****response 174863**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.03
183.00	11.50	11.67
0.00	0.00	0.00