

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121622\
 Data File : BG055993.D
 Acq On : 16 Dec 2022 14:10
 Operator : CG/JU
 Sample : PB149627BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB149627BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG055993.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.415	357	362	368	rBB	14680	21363	1.98%	0.668%
2	5.891	436	443	450	rBB	113874	177738	16.48%	5.560%
3	7.500	710	717	724	rBB	117212	198686	18.42%	6.215%
4	8.376	860	866	871	rBB	19051	30475	2.82%	0.953%
5	9.545	1058	1065	1072	rBB	64284	110906	10.28%	3.469%
6	11.208	1341	1348	1354	rBB	26392	46552	4.32%	1.456%
7	13.611	1750	1757	1763	rBB	273131	416368	38.60%	13.024%
8	14.980	1984	1990	1997	rBB	56907	86374	8.01%	2.702%
9	16.455	2235	2241	2252	rBB	338455	506392	46.94%	15.840%
10	17.718	2450	2456	2462	rVB	98934	145044	13.44%	4.537%
11	20.297	2886	2895	2900	rBV	816375	1078809	100.00%	33.745%
12	22.030	3183	3190	3197	rVB	104099	182673	16.93%	5.714%
13	25.532	3776	3786	3797	rVB	65445	195538	18.13%	6.116%




Sum of corrected areas: 3196918

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121622\
Data File : BG055993.D
Acq On : 16 Dec 2022 14:10
Operator : CG/JU
Sample : PB149627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB149627BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

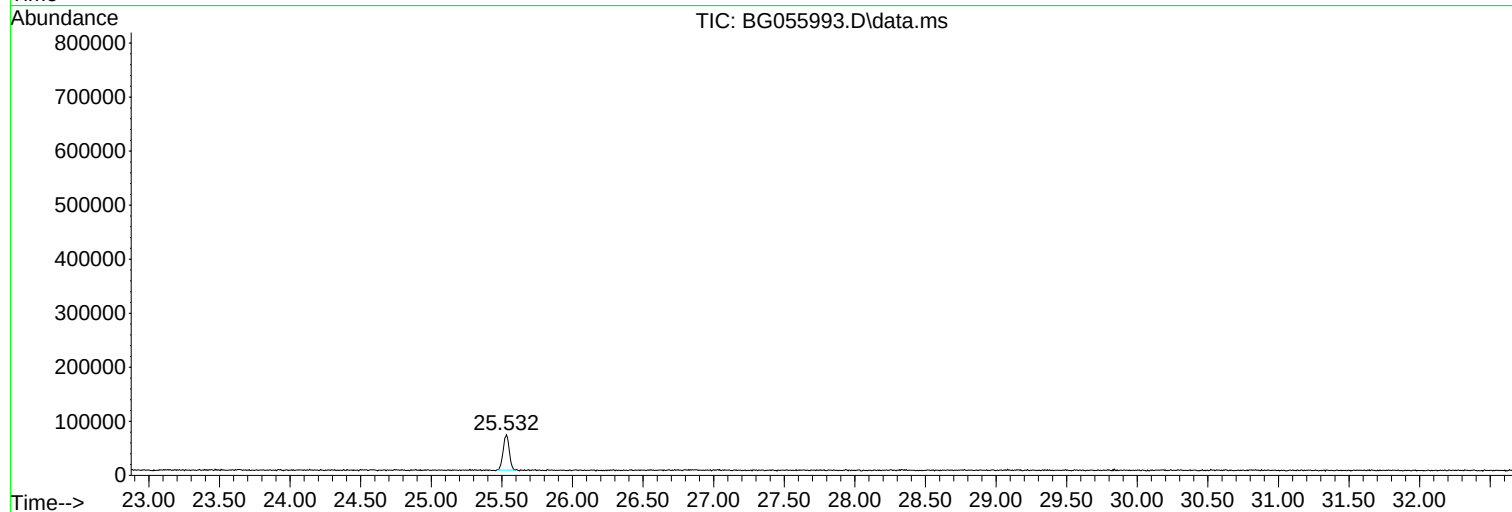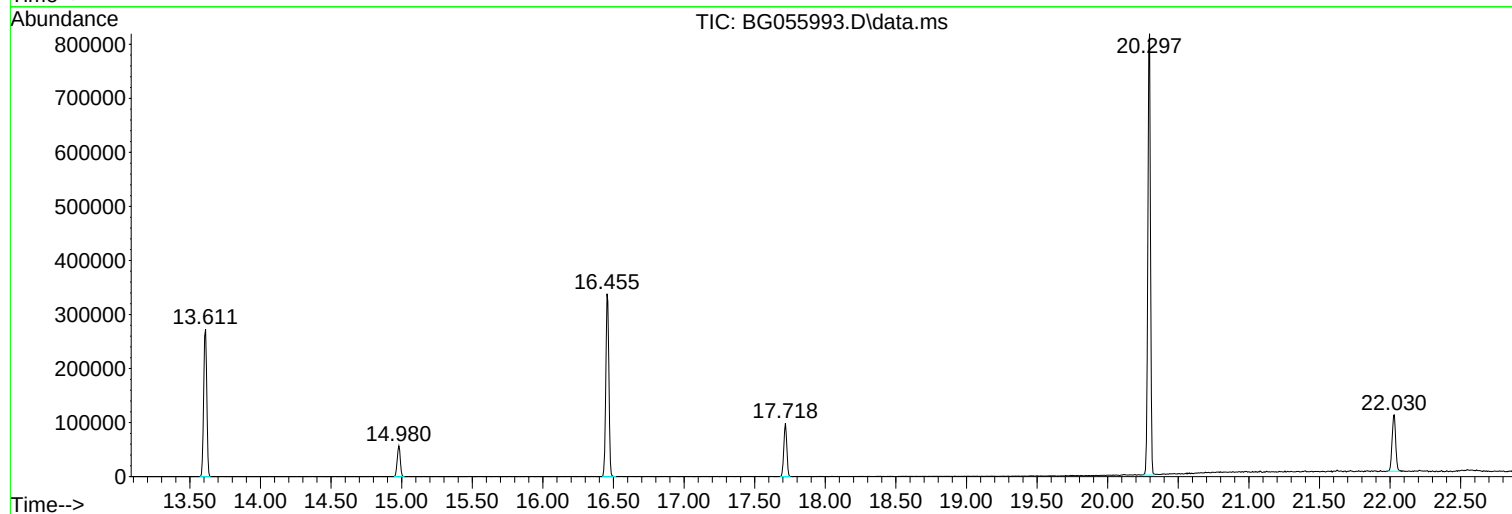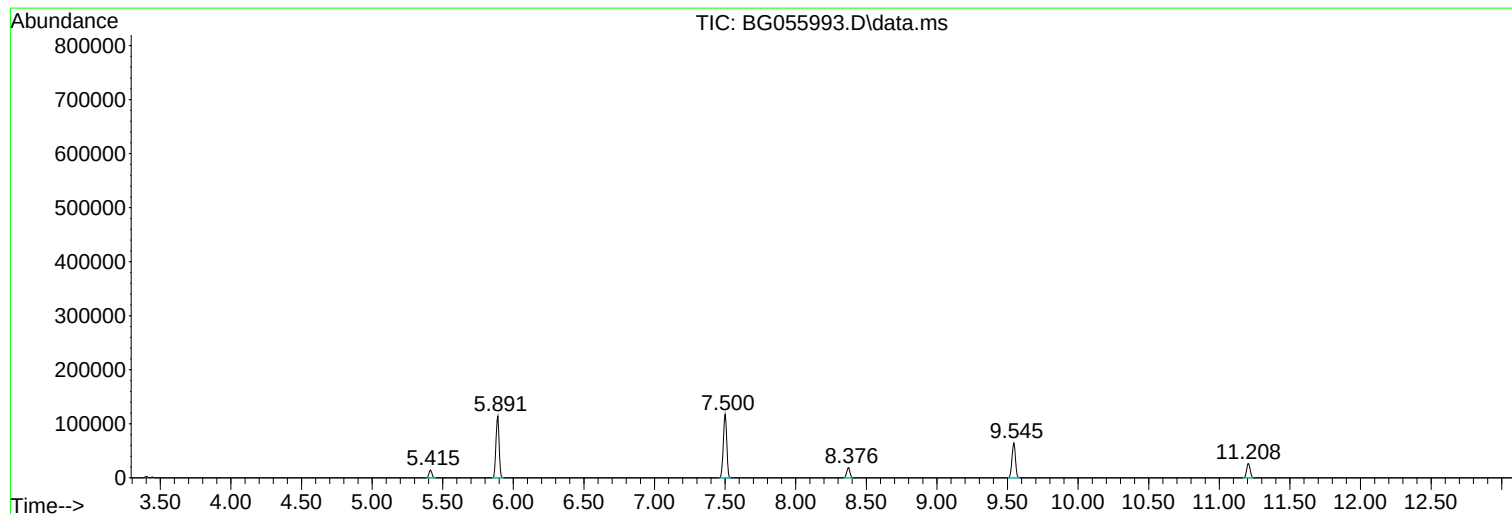

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121622\
Data File : BG055993.D
Acq On : 16 Dec 2022 14:10
Operator : CG/JU
Sample : PB149627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB149627BL









Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.415	14.02 ng	21363	1,4-Dichlorobenzene-d4	8.370

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	2-Nonanone, 9-hydroxy-	158	C9H18O2	025368-56-3	33		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9		
5	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	9		

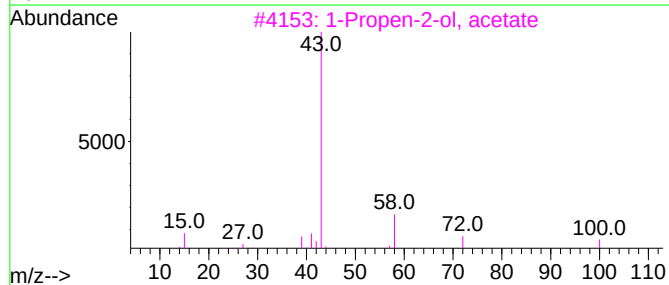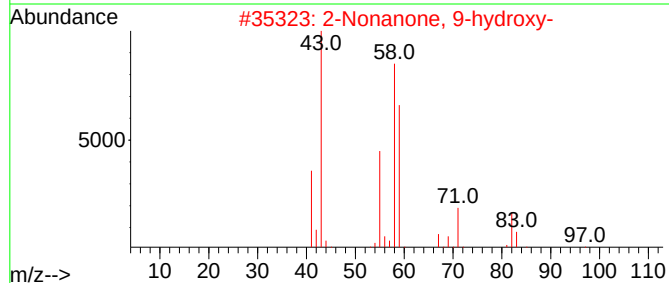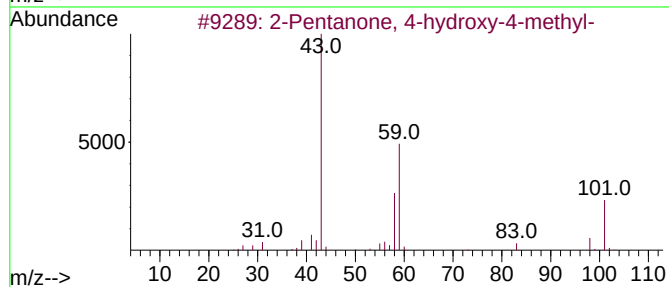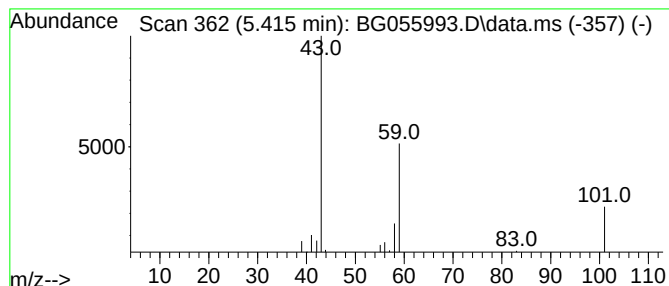

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121622\
Data File : BG055993.D
Acq On : 16 Dec 2022 14:10
Operator : CG/JU
Sample : PB149627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB149627BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.415	14.0	ng	21363	1	8.370	30475	20.0