


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121622\
 Data File : BG055991.D
 Acq On : 16 Dec 2022 12:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 17 01:18:54 2022

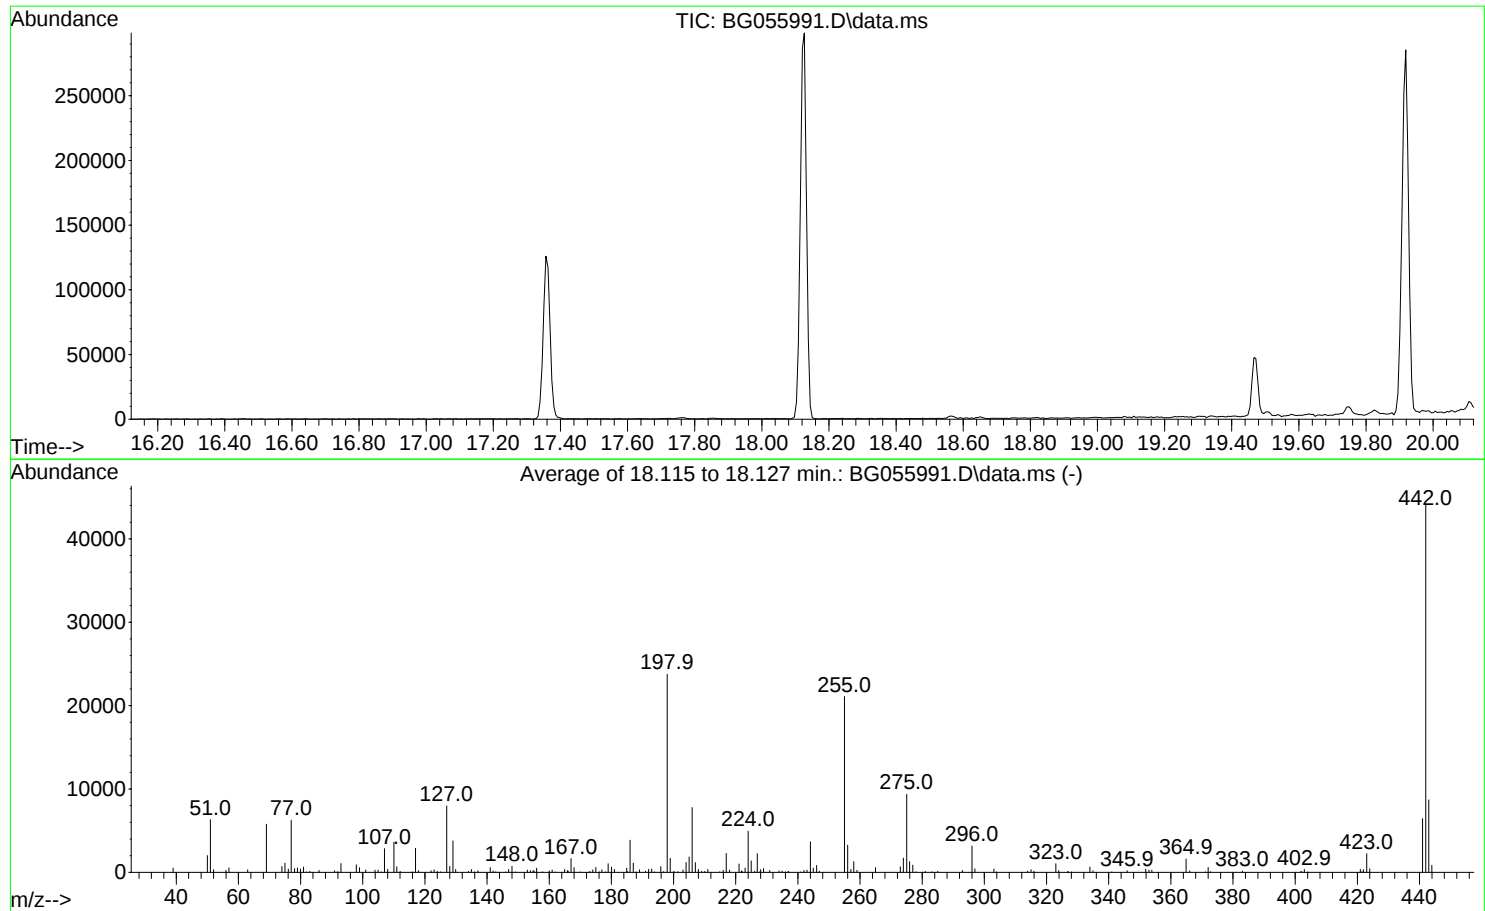

AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.6	6325	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	24.3	5782	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.5	7967	PASS
197	198	0.00	2	0.4	106	PASS
198	198	100	100	100.0	23768	PASS
199	198	5	9	7.1	1694	PASS
275	198	10	60	39.4	9361	PASS
365	198	1	100	6.7	1585	PASS
441	198	0.01	100	27.2	6455	PASS
442	442	50	100	100.0	44123	PASS
443	442	15	24	19.7	8702	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/16/2022	BNA_G	BG055991.D
Compound Name	Response	Retention Time
DDT	78610	21.164
DDD	2709	20.709
DDE	0	20.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2709	81319	3.33

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121622\
Data File : BG055991.D
Acq On : 16 Dec 2022 12:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 17 06:16:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 01:18:54 2022
Response via : Initial Calibration

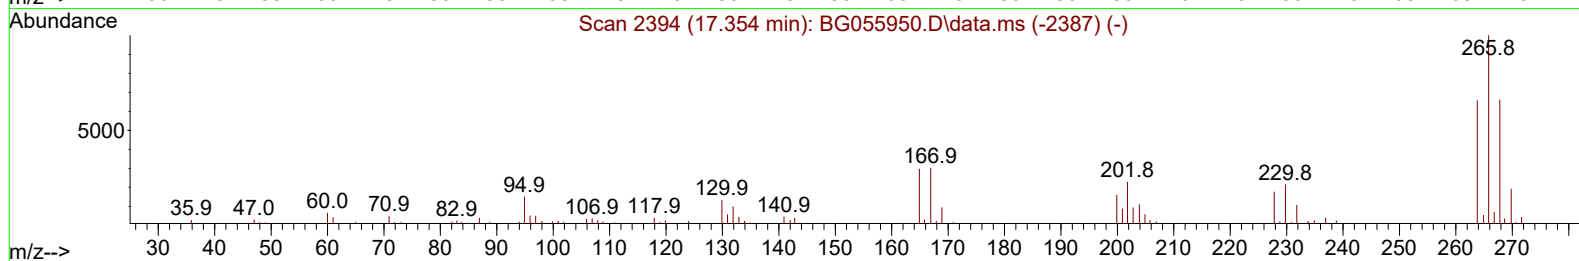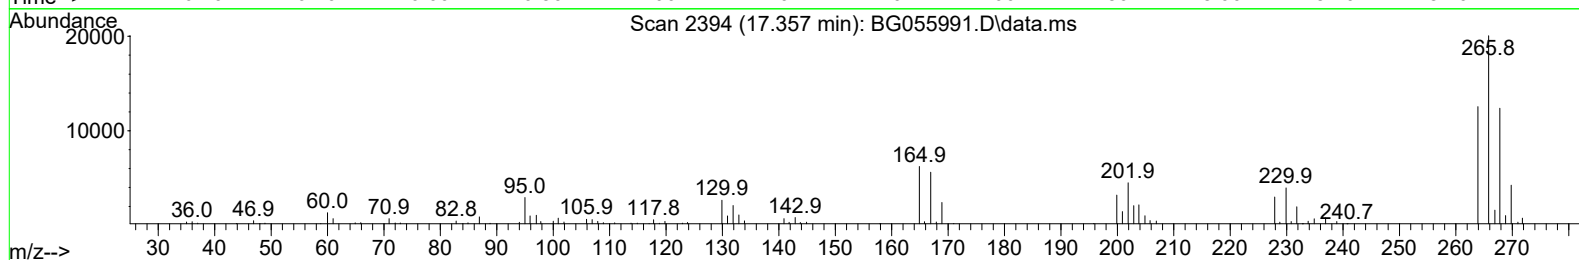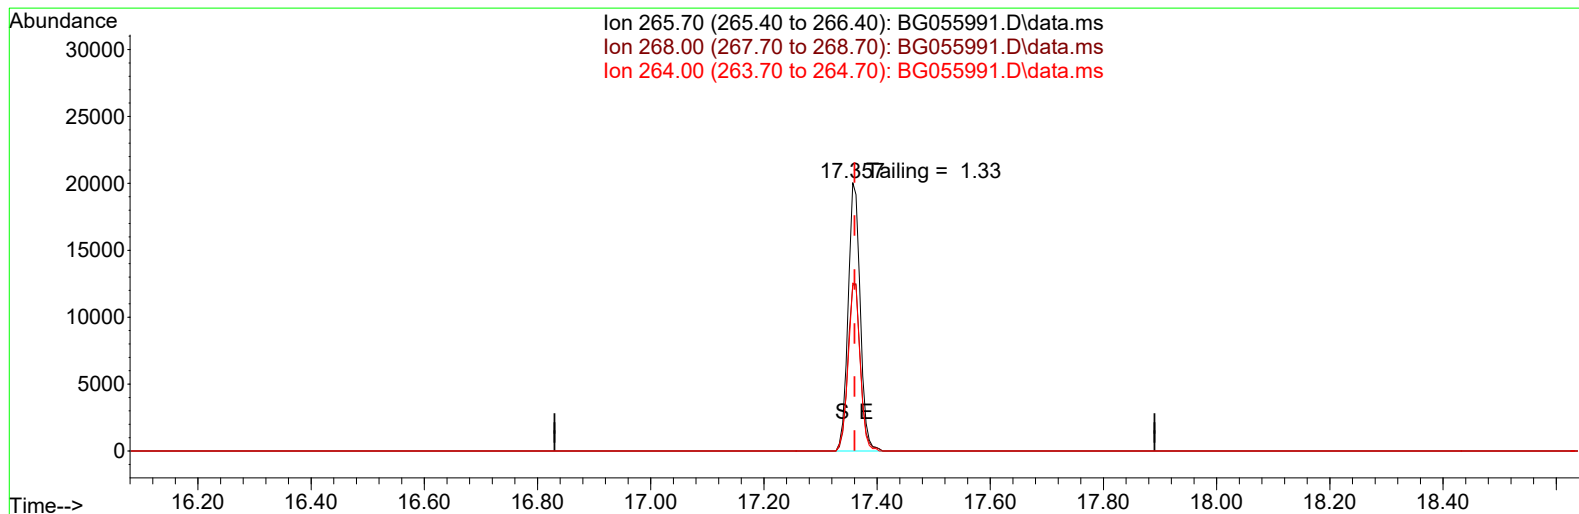

TIC: BG055991.D\data.ms

(70) Pentachlorophenol (C)

17.357min (-0.003) 6069.53 ng


response 29623

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.40	61.81
264.00	65.70	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121622\
Data File : BG055991.D
Acq On : 16 Dec 2022 12:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 17 06:16:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 01:18:54 2022
Response via : Initial Calibration

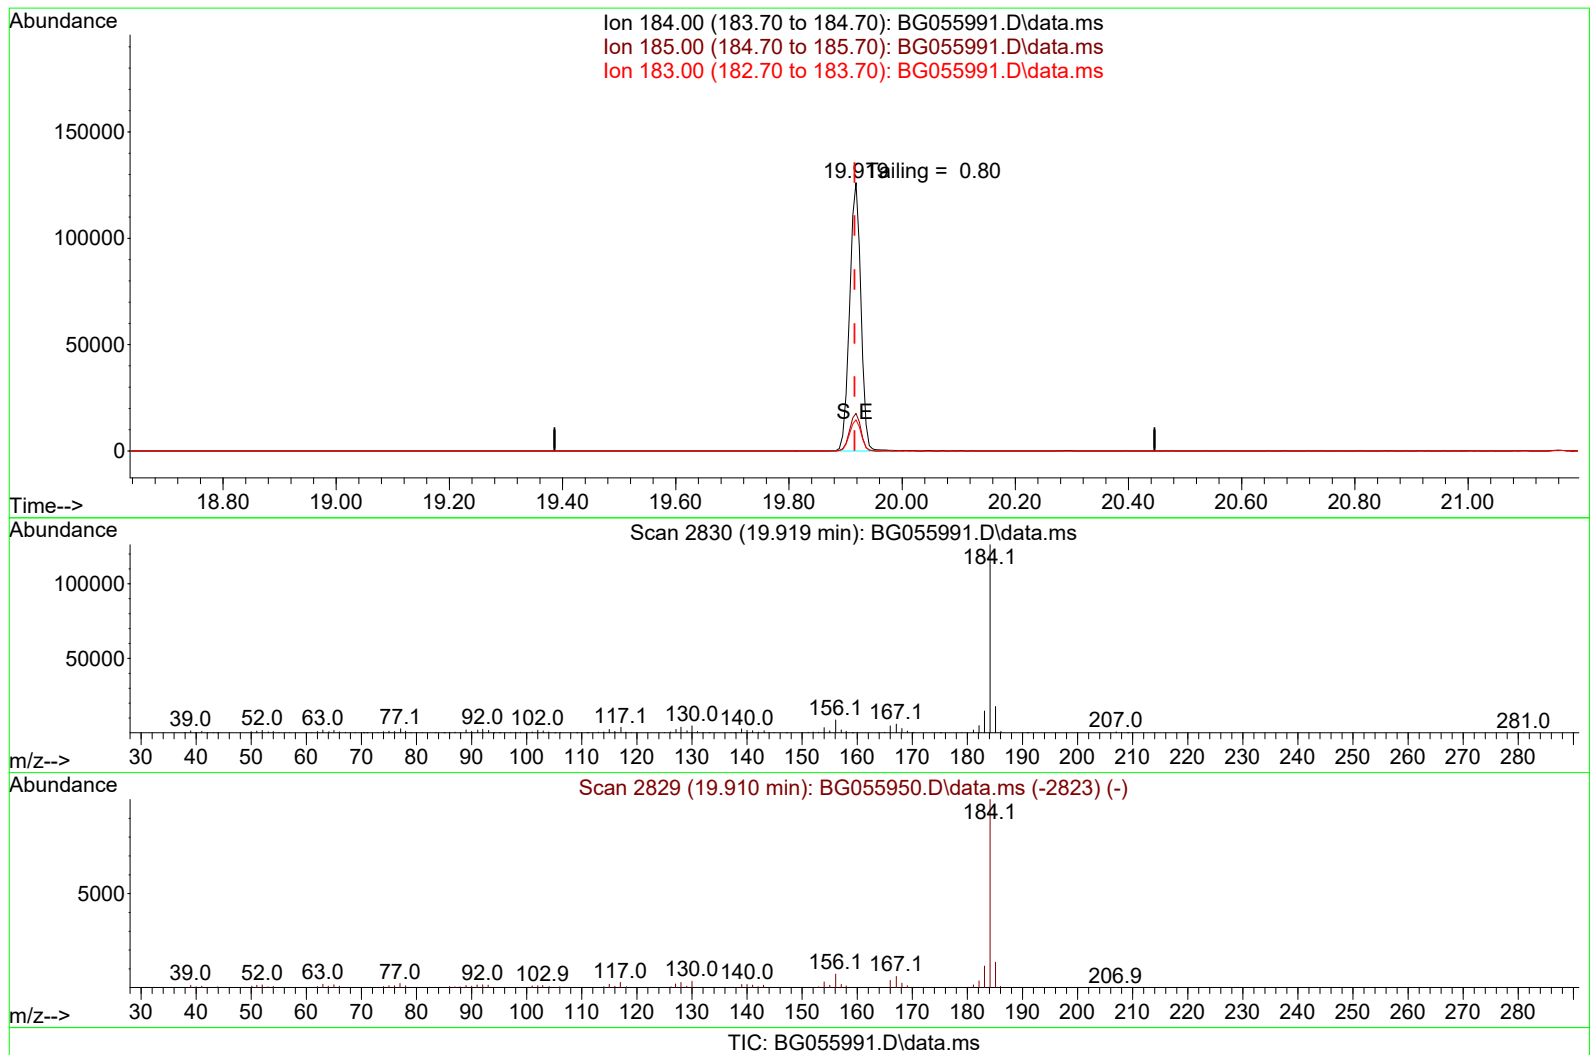

(77) Benzidine

19.919min (+ 0.003) 13015.78 ng

response 174863

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.03
183.00	11.50	11.67
0.00	0.00	0.00