
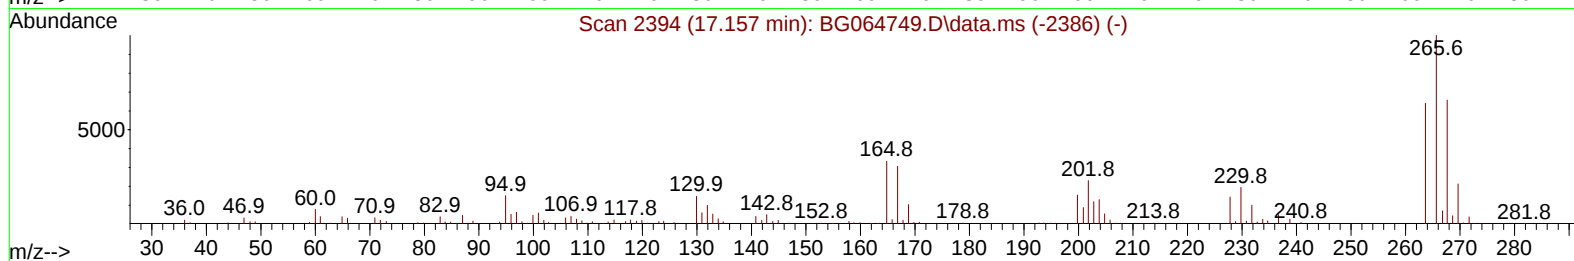
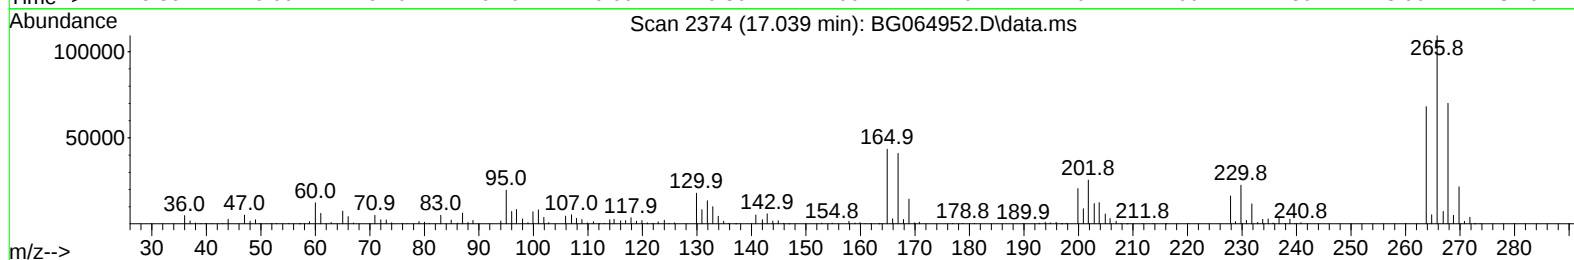


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121625\
Data File : BG064952.D
Acq On : 16 Dec 2025 11:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 14:27:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 16 14:12:58 2025
Response via : Initial Calibration

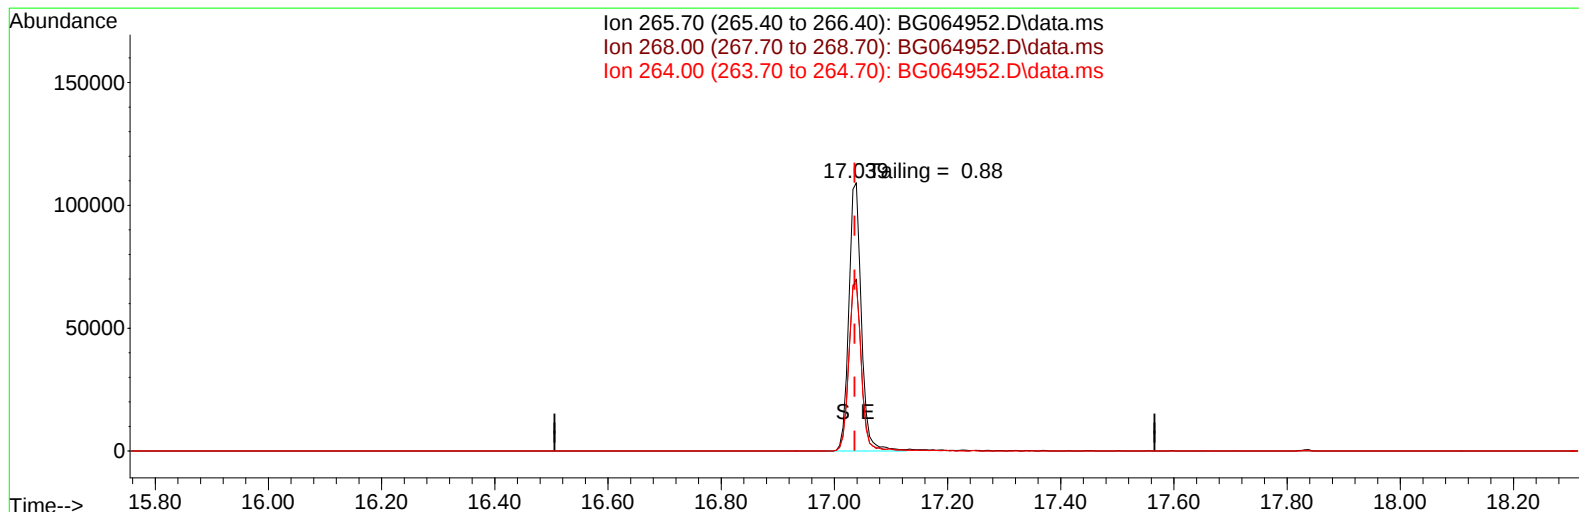

TIC: BG064952.D\data.ms

(70) Pentachlorophenol (C)




17.039min (+ 0.003) 24466.91 ng

response 167647

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.10	64.13
264.00	64.00	62.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121625\
Data File : BG064952.D
Acq On : 16 Dec 2025 11:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 14:27:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 16 14:12:58 2025
Response via : Initial Calibration

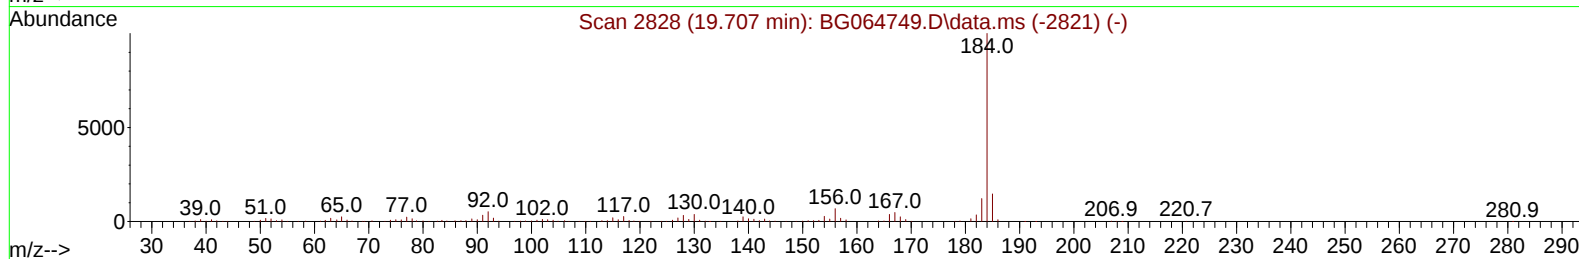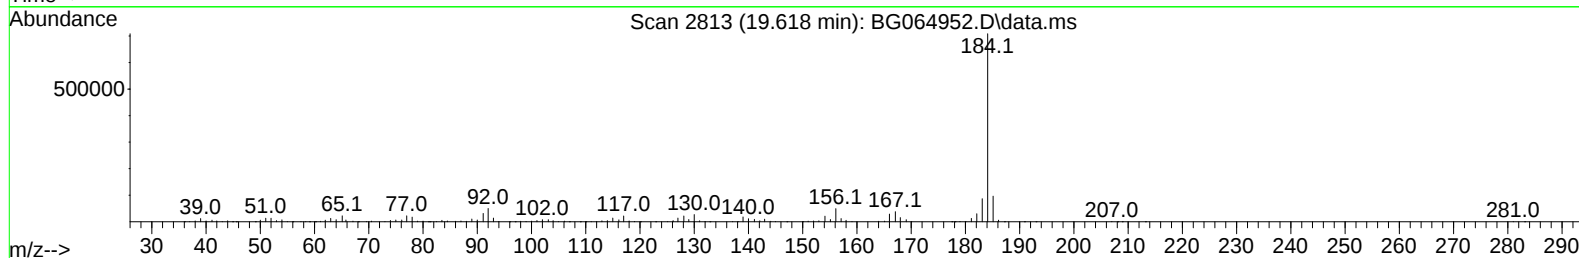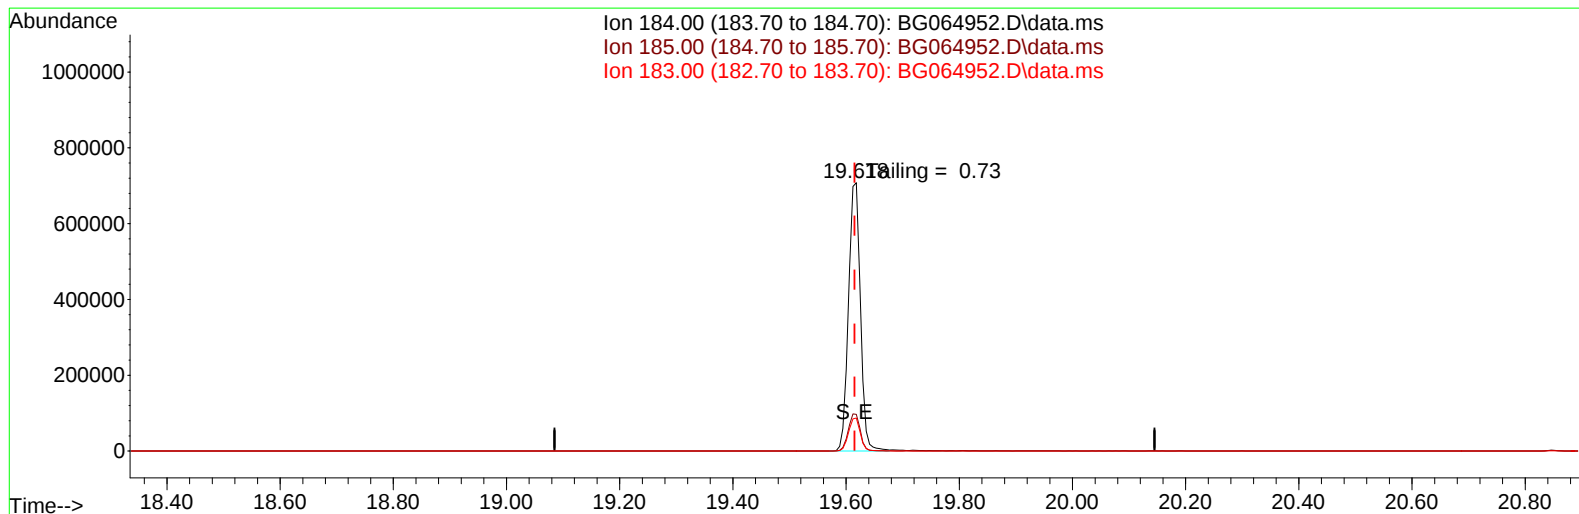

TIC: BG064952.D\data.ms

(77) Benzidine

19.618min (+ 0.003) 0.00 ng

response 1036619

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.66
183.00	12.20	12.31
0.00	0.00	0.00