


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121625\
Data File : BG064952.D
Acq On : 16 Dec 2025 11:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 17 05:53:31 2025

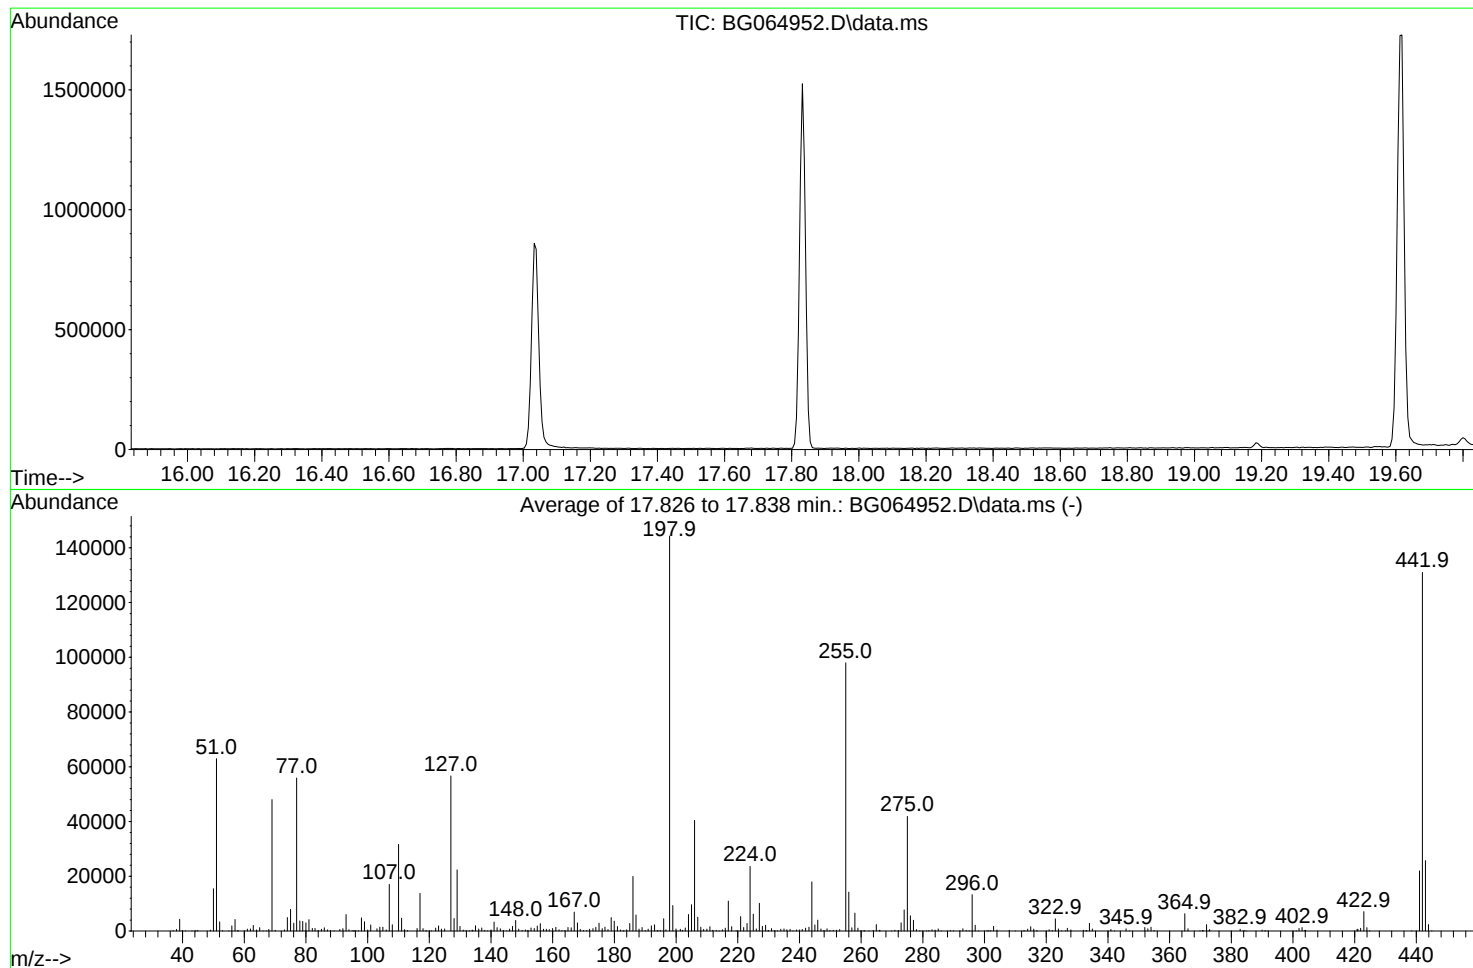




AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.2	576	PASS
69	69	100	100	100.0	47968	PASS
70	69	0.00	2	0.6	291	PASS
197	198	0.00	2	0.3	432	PASS
198	198	100	100	100.0	144248	PASS
199	198	5	9	6.5	9307	PASS
365	198	1	100	4.4	6290	PASS
441	443	0.01	150	85.4	21954	PASS
442	442	100	100	100.0	131011	PASS
443	442	15	24	19.6	25720	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121625\
Data File : BG064952.D
Acq On : 16 Dec 2025 11:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 16 14:27:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 16 14:12:58 2025
Response via : Initial Calibration

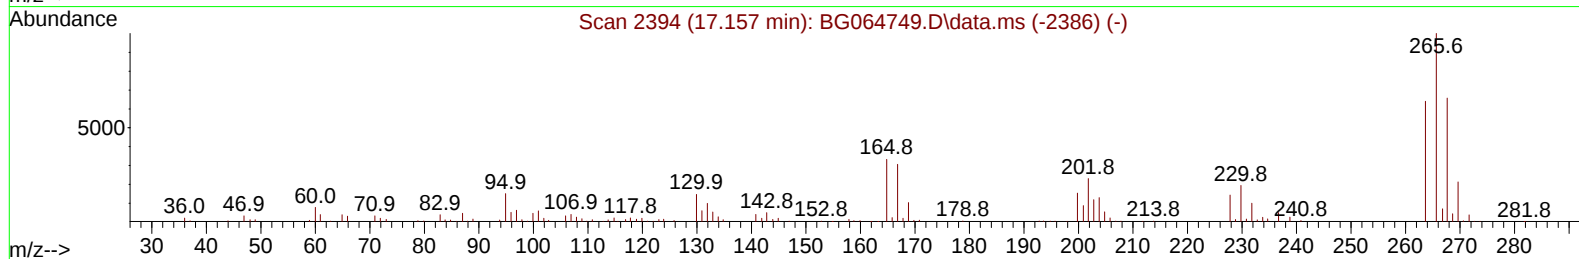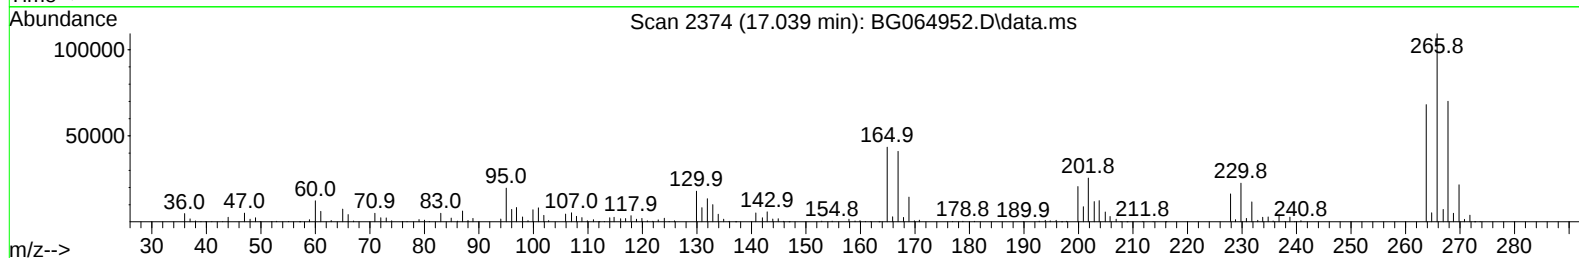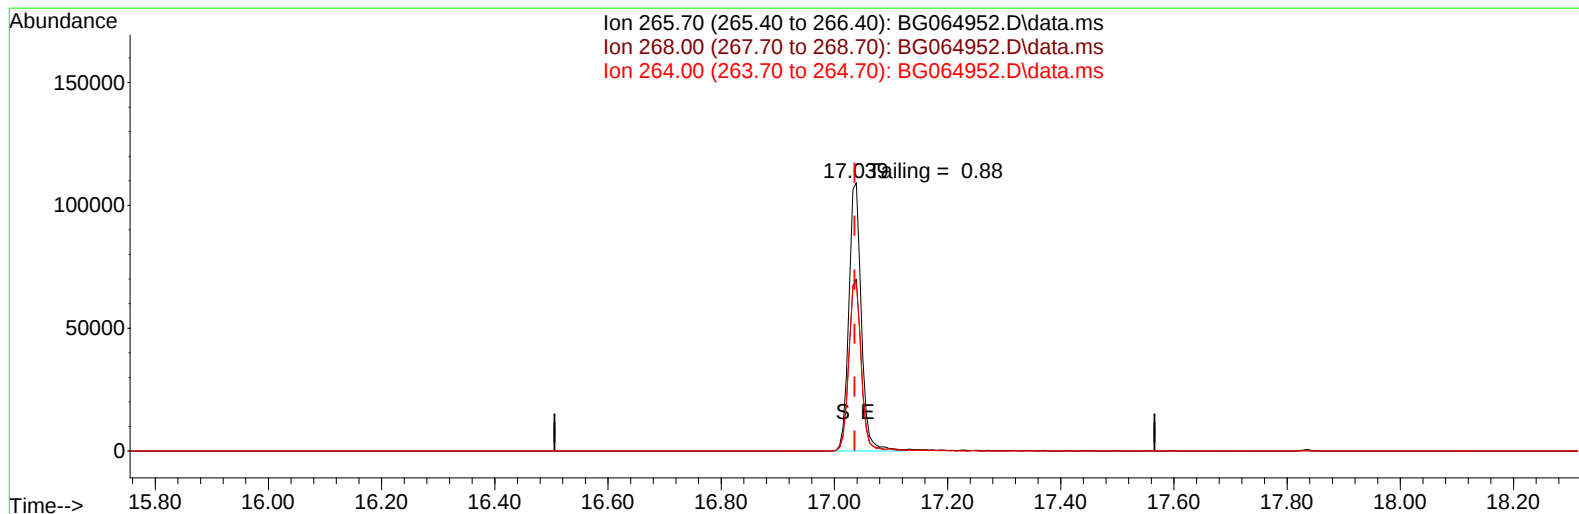

TIC: BG064952.D\data.ms

(70) Pentachlorophenol (C)

17.039min (+ 0.003) 24466.91 ng




response 167647

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.10	64.13
264.00	64.00	62.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121625\
Data File : BG064952.D
Acq On : 16 Dec 2025 11:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 16 14:27:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 16 14:12:58 2025
Response via : Initial Calibration

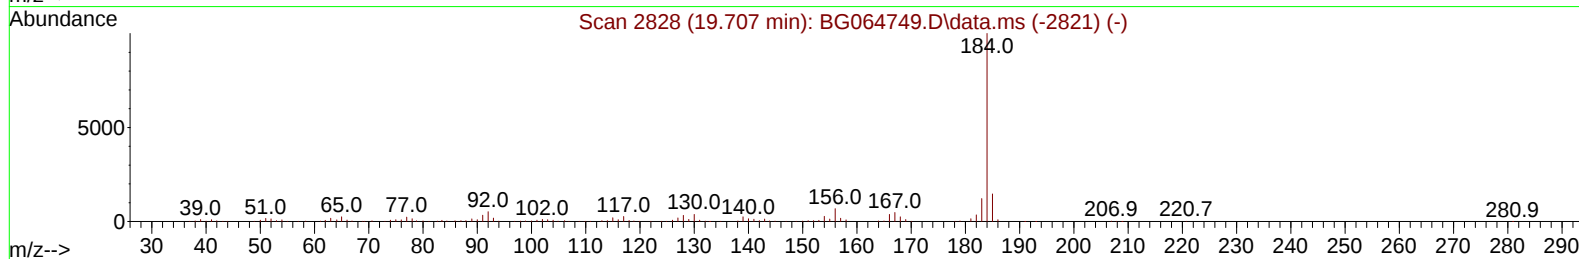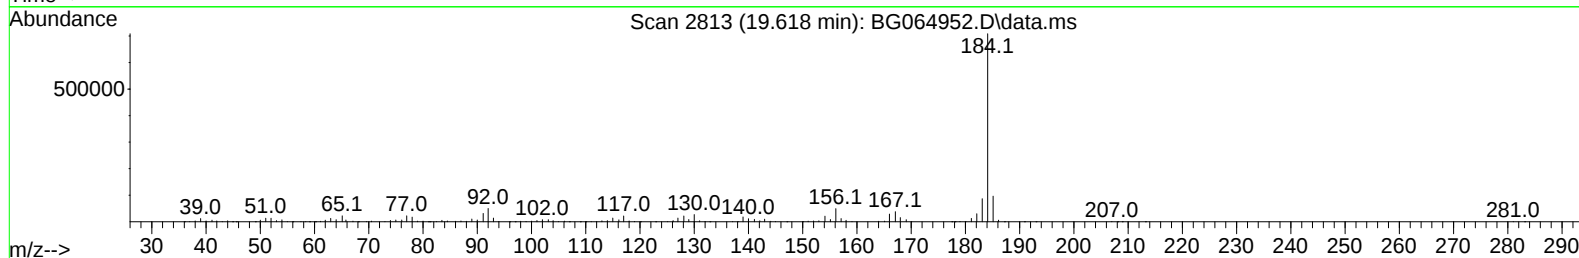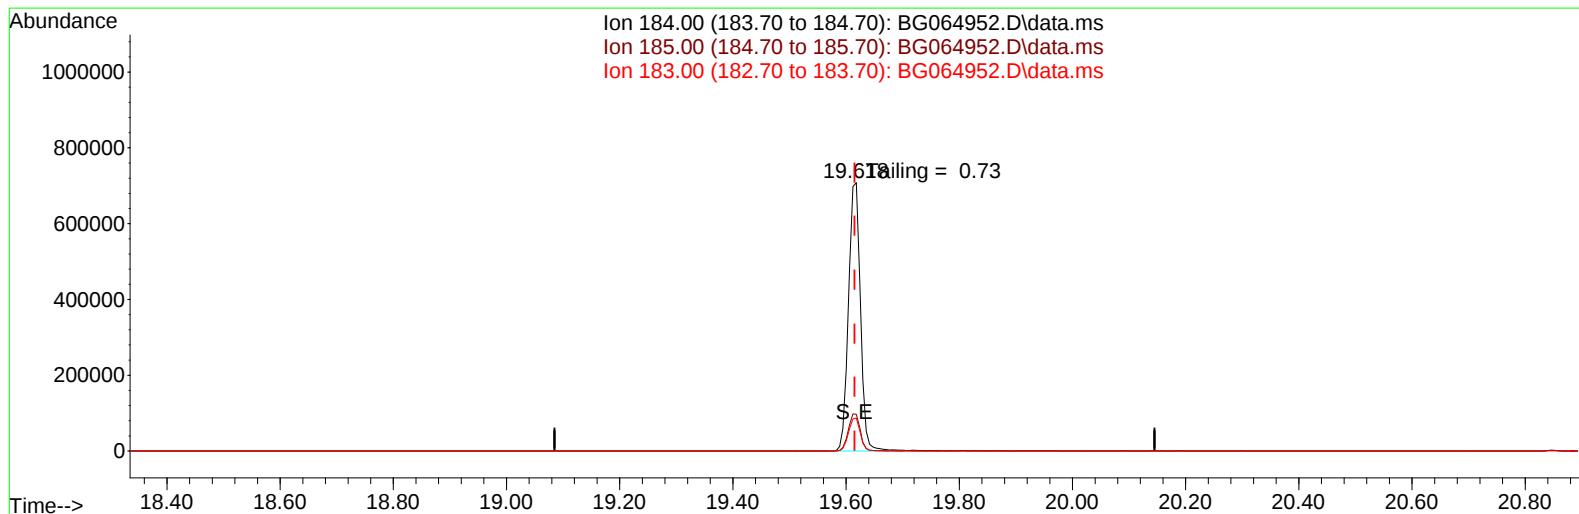

TIC: BG064952.D\data.ms

(77) Benzidine

19.618min (+ 0.003) 0.00 ng

response 1036619

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.66
183.00	12.20	12.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/16/2025	BNA_G	<u>BG064952.D</u>
Compound Name	Response	Retention Time
DDT	400512	20.852
DDD	8504	20.405
DDE	361	19.906
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8865	409377	2.17

Instrument :
BNA_G
ClientSampleId :
DFTPP