

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG121718\
 Data File : BG038659.D
 Acq On : 17 Dec 2018 12:25
 Operator : JU/SJ
 Sample : J6379-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P001-SS004-1824-01

Quant Time: Dec 18 03:17:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 12 15:26:27 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	20726	20.00	ng	0.00
21) Naphthalene-d8	10.88	136	82662	20.00	ng	0.00
39) Acenaphthene-d10	14.70	164	54955	20.00	ng	0.00
64) Phenanthrene-d10	17.44	188	152719	20.00	ng	0.00
76) Chrysene-d12	21.72	240	169447	20.00	ng	0.00
87) Perylene-d12	25.02	264	176580	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	189493	162.16	ng	0.00
7) Phenol-d6	7.21	99	257892	160.76	ng	0.00
23) Nitrobenzene-d5	9.24	82	173140	107.00	ng	0.00
42) 2,4,6-Tribromophenol	16.19	330	134952	178.18	ng	0.00
45) 2-Fluorobiphenyl	13.32	172	374963	93.60	ng	0.00
79) Terphenyl-d14	20.04	244	775188	99.56	ng	0.00
Target Compounds						
10) Phenol	7.24	94	16275	9.549	ng	97
50) Dimethylphthalate	14.14	163	34334	7.650	ng	# 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG121718\
Data File : BG038659.D
Acq On : 17 Dec 2018 12:25
Operator : JU/SJ
Sample : J6379-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P001-SS004-1824-01

Quant Time: Dec 18 03:17:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

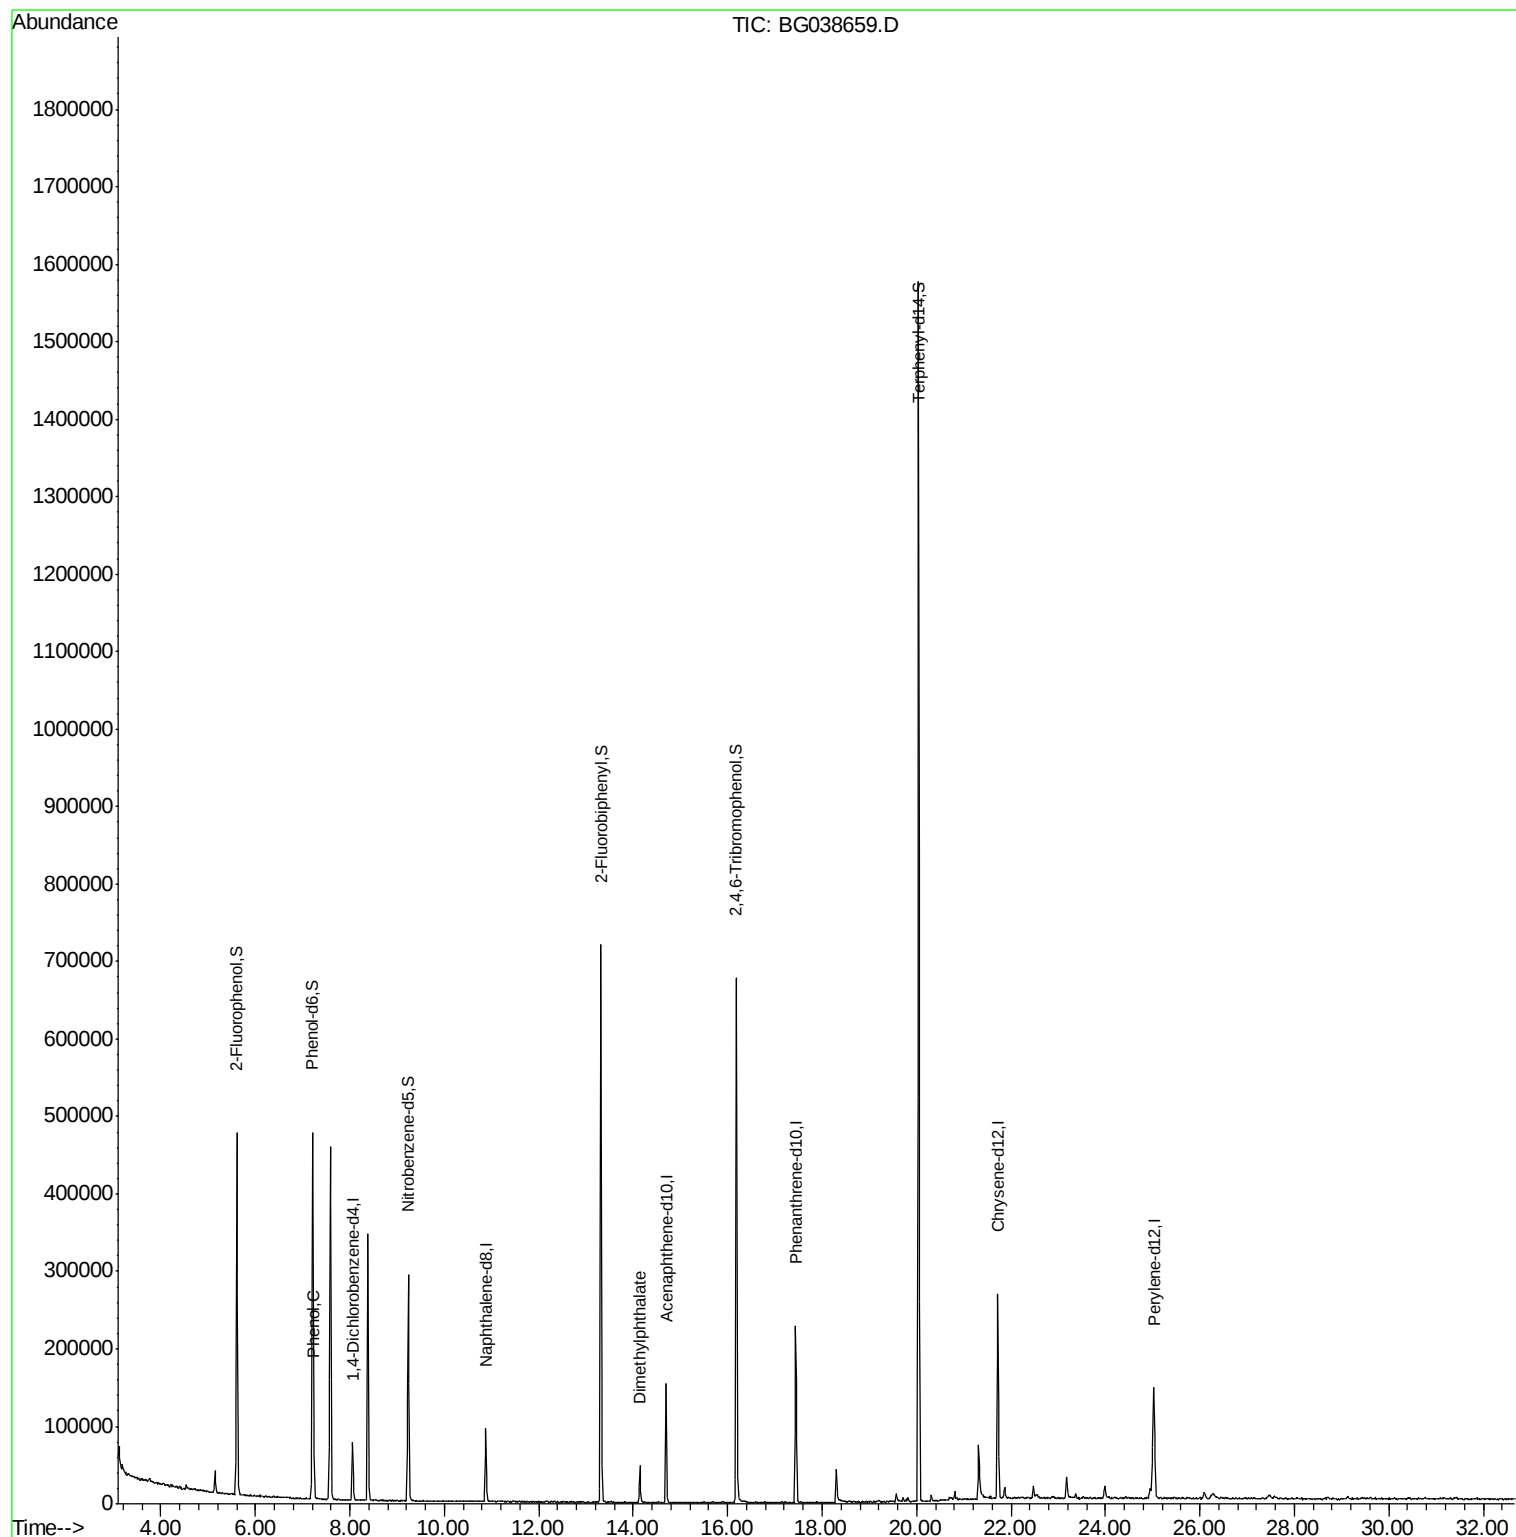




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.06 min Scan# 846
Delta R.T. -0.00 min
Lab File: BG038659.D
Acq: 17 Dec 2018 12:25

Instrument :
BNA_G
ClientSampleId :
P001-SS004-1824-01

Tgt Ion:152 Resp: 20726
Ion Ratio Lower Upper
152 100
150 158.7 119.5 179.3
115 58.1 49.6 74.4

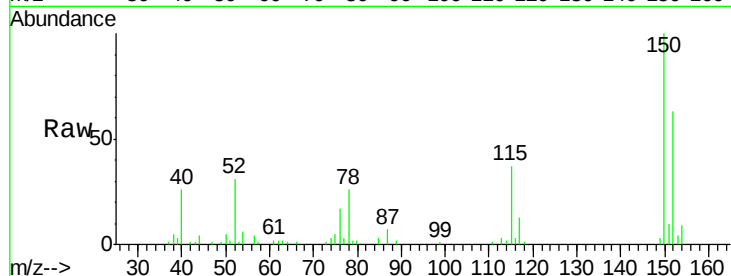


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

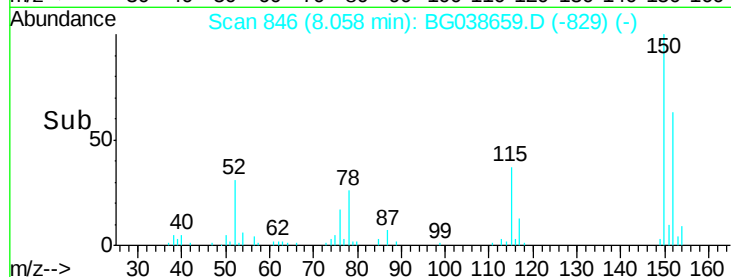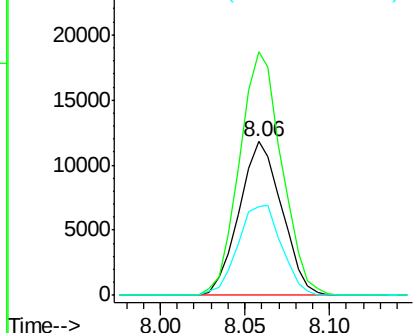



#5

2-Fluorophenol
Concen: 162.161 ng
RT: 5.61 min Scan# 429
Delta R.T. 0.00 min
Lab File: BG038659.D
Acq: 17 Dec 2018 12:25

Tgt Ion:112 Resp: 189493
Ion Ratio Lower Upper
112 100
64 71.0 53.4 80.2
63 40.1 29.3 43.9

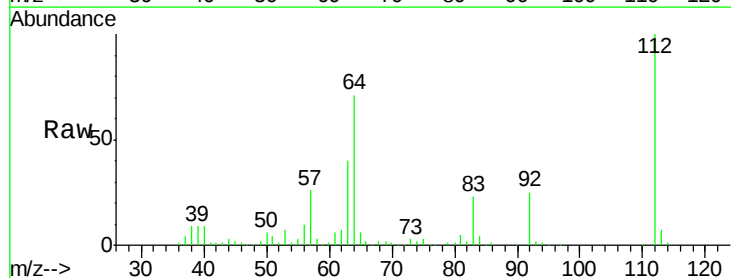

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

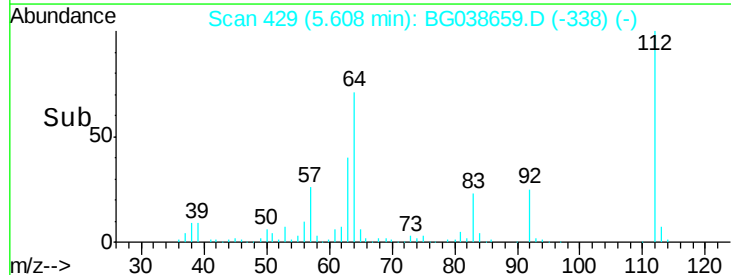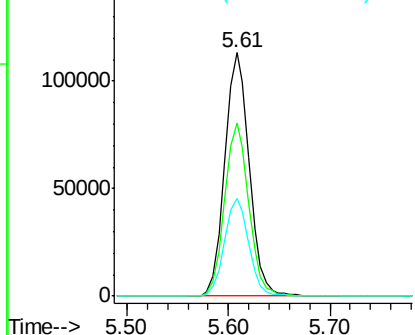



#7

Phenol-d6

Concen: 160.761 ng

RT: 7.21 min Scan# 702

Delta R.T. 0.00 min

Lab File: BG038659.D

Acq: 17 Dec 2018 12:25

Instrument :

BNA_G

ClientSampleId :

P001-SS004-1824-01


Tgt Ion: 99 Resp: 257892

Ion Ratio Lower Upper




99 100

42 25.1 18.5 27.7

71 41.1 31.1 46.7

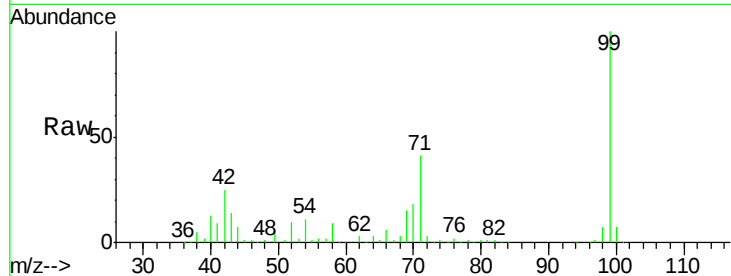

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

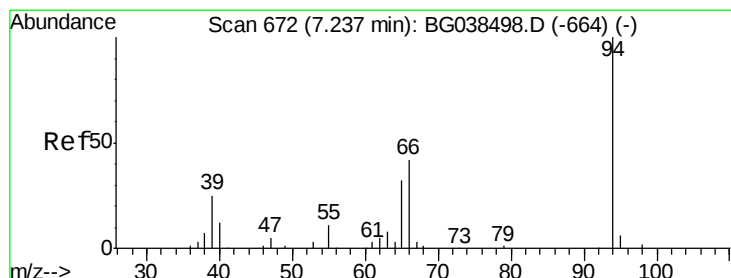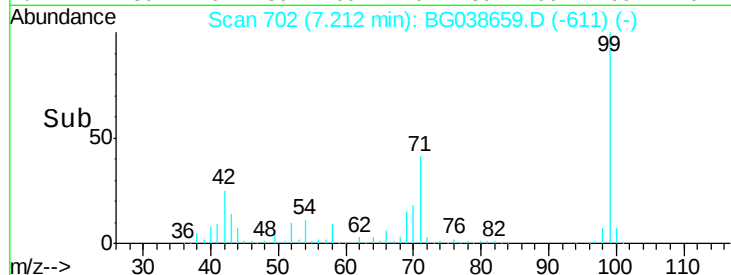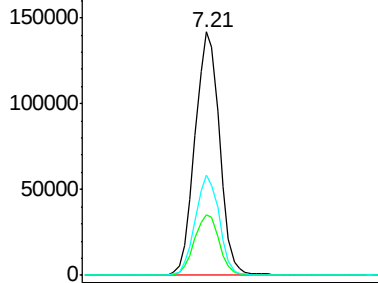

#10

Phenol

Concen: 9.549 ng

RT: 7.24 min Scan# 707

Delta R.T. 0.00 min

Lab File: BG038659.D

Acq: 17 Dec 2018 12:25


Tgt Ion: 94 Resp: 16275

Ion Ratio Lower Upper



94 100

65 35.9 12.6 52.6

66 45.2 24.1 64.1

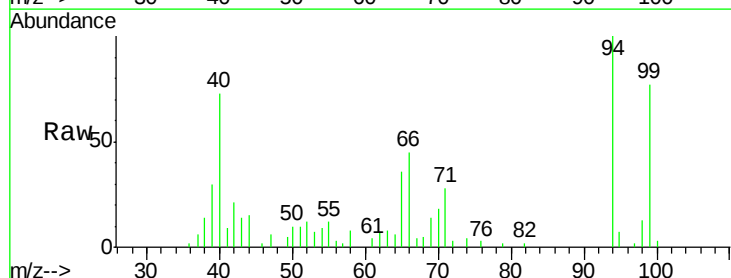

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

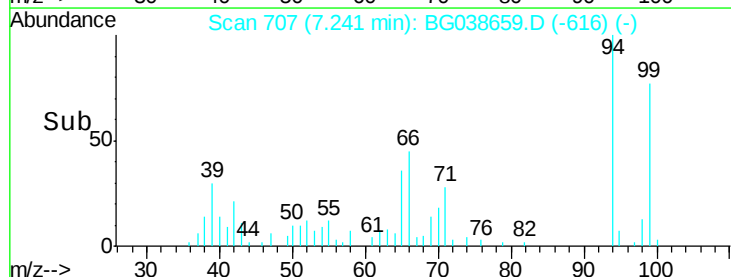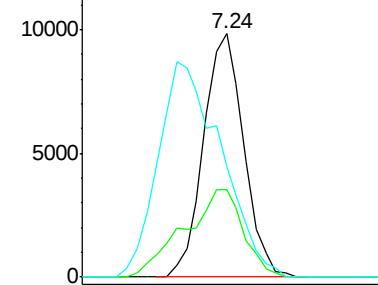







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.88 min Scan# 1326
Delta R.T. -0.00 min
Lab File: BG038659.D
Acq: 17 Dec 2018 12:25

Instrument :
BNA_G
ClientSampleId :
P001-SS004-1824-01

Tgt Ion: 136 Resp: 82662
Ion Ratio Lower Upper
136 100
137 12.0 9.3 13.9
54 11.4 8.5 12.7
68 4.8 3.5 5.3

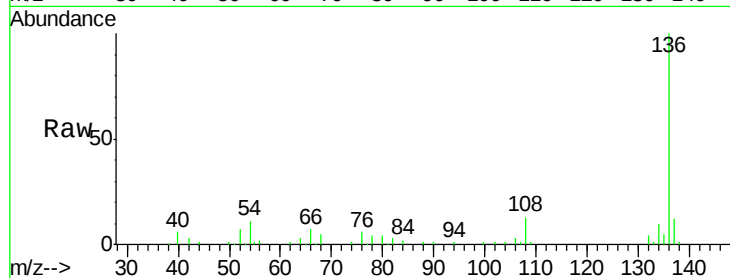


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

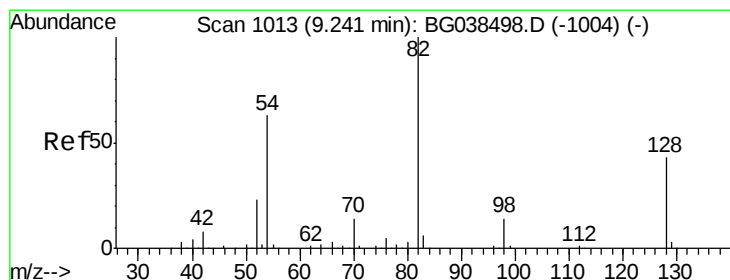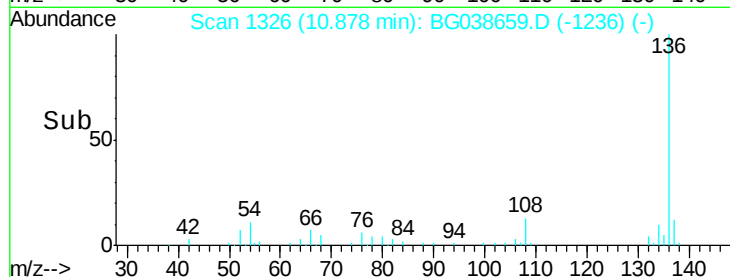
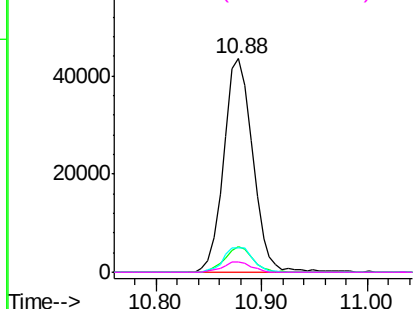


#23
Nitrobenzene-d5
Concen: 107.005 ng
RT: 9.24 min Scan# 1047
Delta R.T. -0.00 min
Lab File: BG038659.D
Acq: 17 Dec 2018 12:25

Tgt Ion: 82 Resp: 173140
Ion Ratio Lower Upper
82 100
128 40.9 34.6 52.0
54 64.5 50.6 76.0

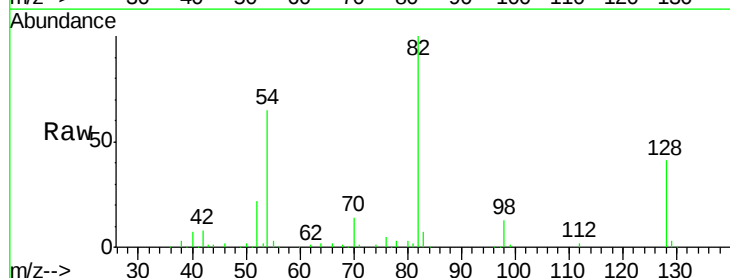

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

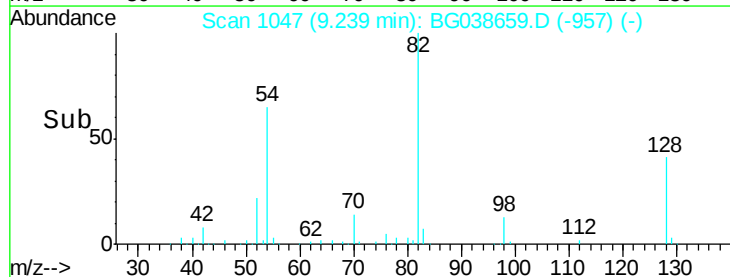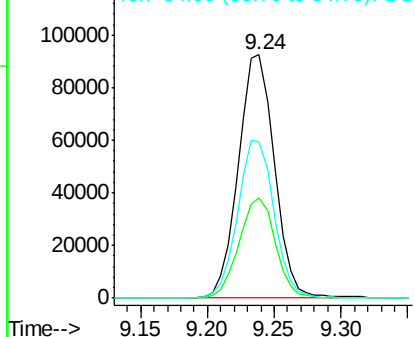



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.70 min Scan# 1976

Delta R.T. -0.00 min

Lab File: BG038659.D

Acq: 17 Dec 2018 12:25

Instrument :

BNA_G

ClientSampleId :

P001-SS004-1824-01


Tgt Ion:164 Resp: 54955

Ion Ratio Lower Upper

164 100

162 105.3 86.6 130.0




160 46.0 34.2 51.2

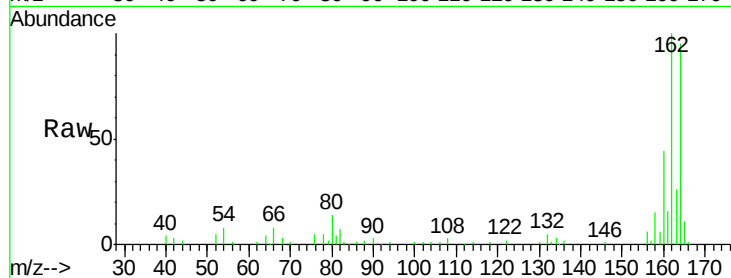

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

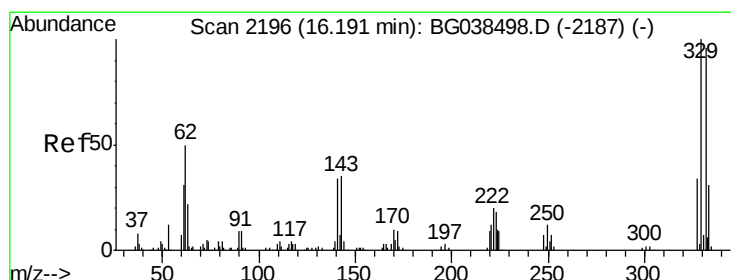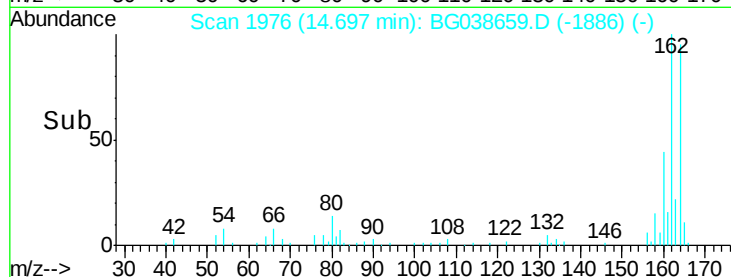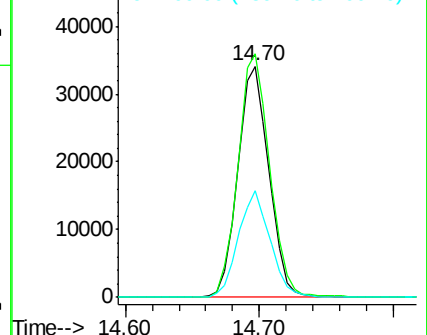

#42

2,4,6-Tribromophenol

Concen: 178.183 ng

RT: 16.19 min Scan# 2230

Delta R.T. -0.00 min

Lab File: BG038659.D

Acq: 17 Dec 2018 12:25


Tgt Ion:330 Resp: 134952

Ion Ratio Lower Upper

330 100

332 95.6 76.9 115.3



141 37.6 28.8 43.2

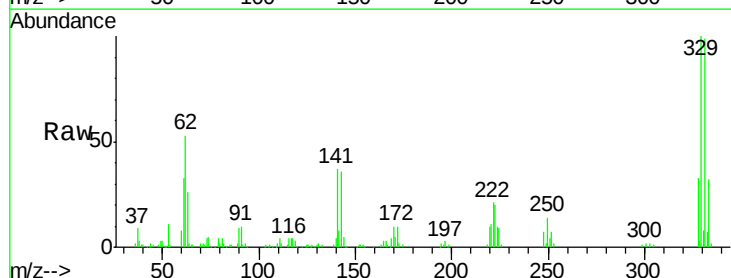

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



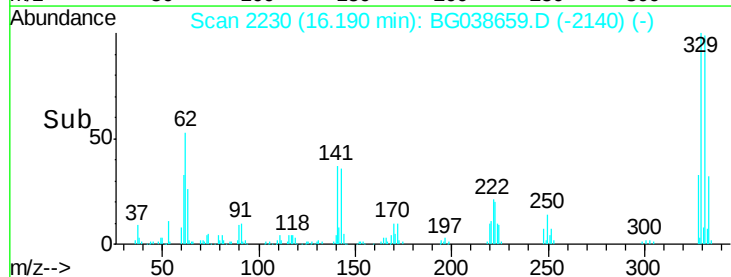
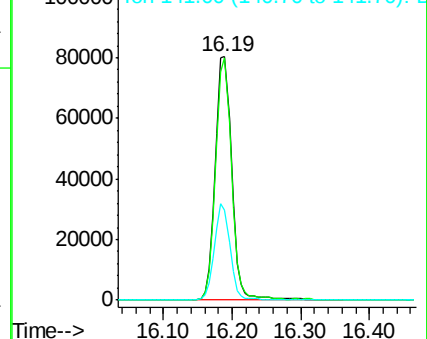




#45
 2-Fluorobiphenyl
 Concen: 93.602 ng
 RT: 13.32 min Scan# 1741
 Delta R.T. -0.00 min
 Lab File: BG038659.D
 Acq: 17 Dec 2018 12:25




Instrument :
 BNA_G
 ClientSampleId :
 P001-SS004-1824-01


Tgt Ion:172 Resp: 374963
 Ion Ratio Lower Upper
 172 100
 171 36.7 29.8 44.6
 170 25.0 19.5 29.3

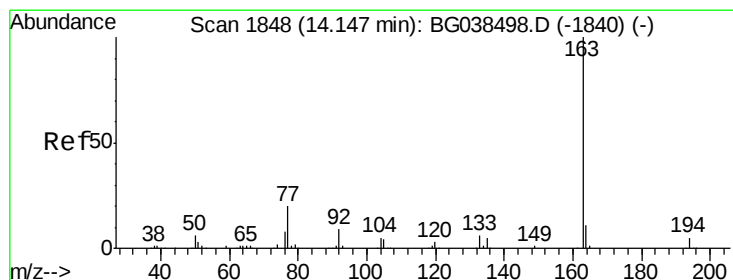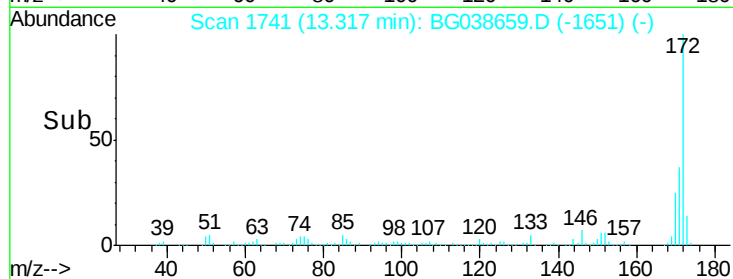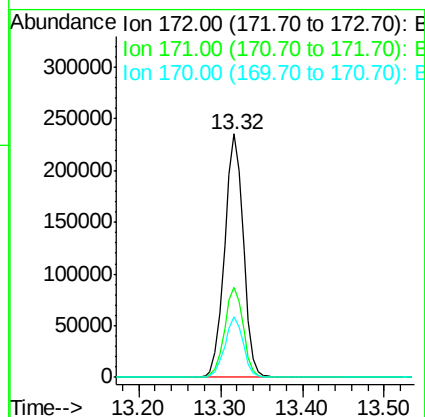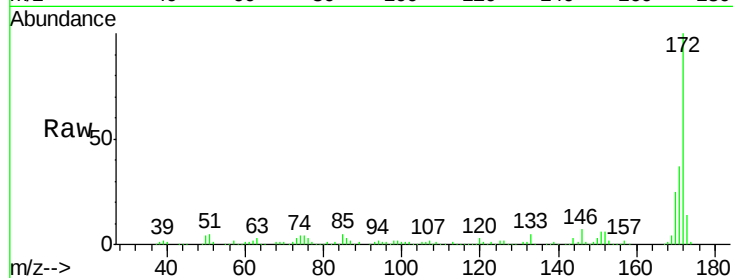

#50
 Dimethylphthalate
 Concen: 7.650 ng
 RT: 14.14 min Scan# 1881
 Delta R.T. -0.01 min
 Lab File: BG038659.D
 Acq: 17 Dec 2018 12:25

Tgt Ion:163 Resp: 34334
 Ion Ratio Lower Upper
 163 100
 194 5.6 3.7 5.5#
 164 11.3 8.6 12.8

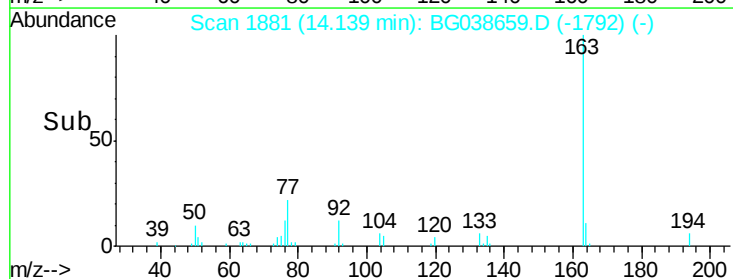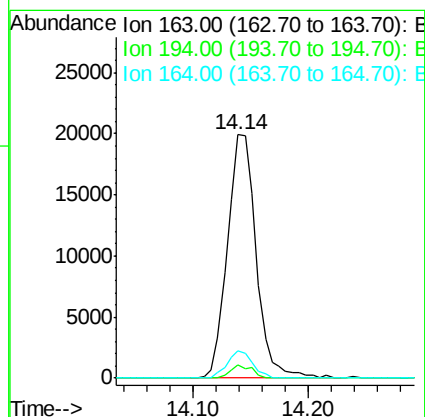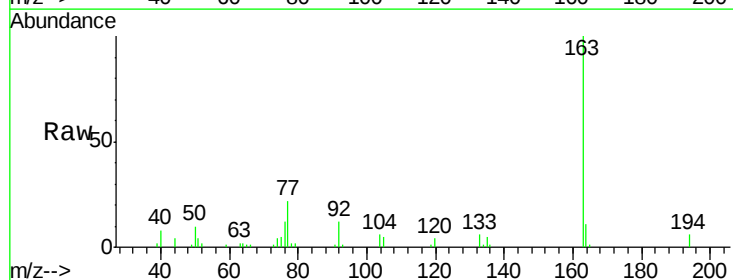


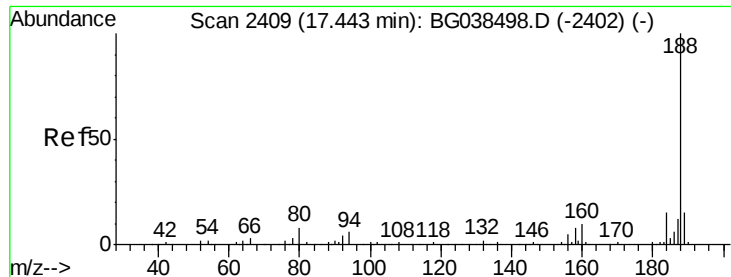




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.44 min Scan# 2443
Delta R.T. -0.00 min
Lab File: BG038659.D
Acq: 17 Dec 2018 12:25

Instrument :
BNA_G
ClientSampleId :
P001-SS004-1824-01

Tgt Ion:188 Resp: 152719
Ion Ratio Lower Upper
188 100
94 6.7 5.1 7.7
80 7.7 6.1 9.1

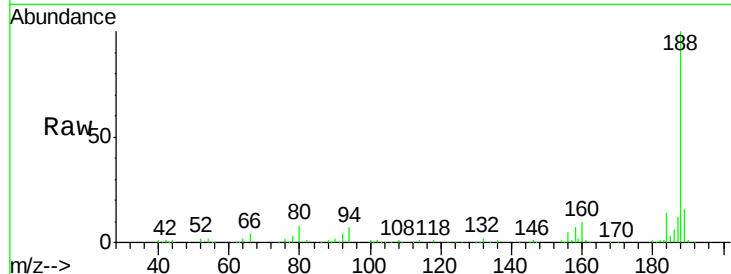


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGO
Ion 80.00 (79.70 to 80.70): BGO

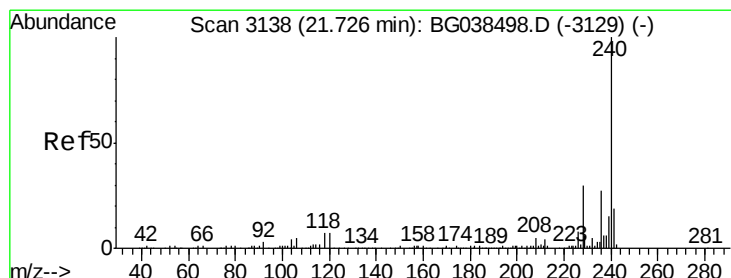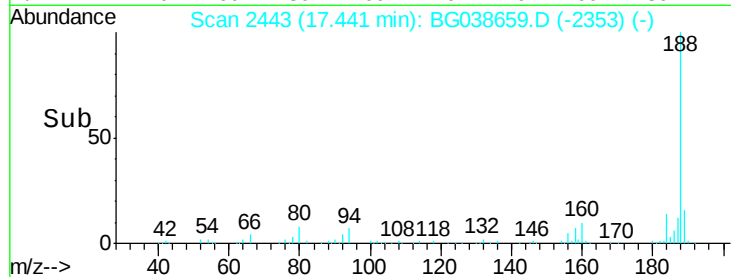
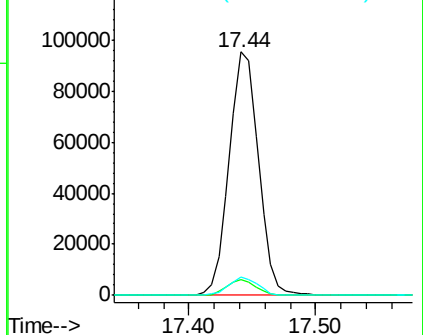



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.72 min Scan# 3172
Delta R.T. -0.00 min
Lab File: BG038659.D
Acq: 17 Dec 2018 12:25

Tgt Ion:240 Resp: 169447
Ion Ratio Lower Upper
240 100
120 6.7 5.3 7.9
236 26.8 21.4 32.2

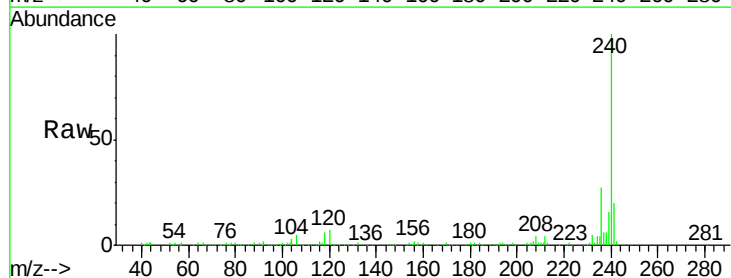

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

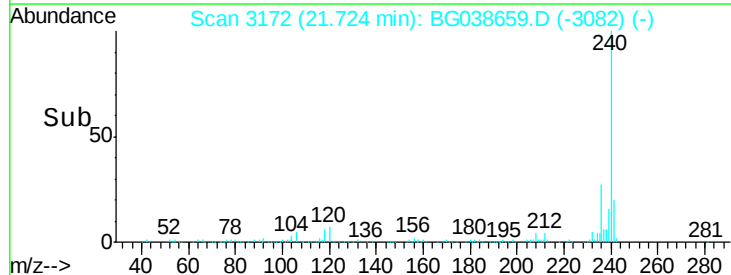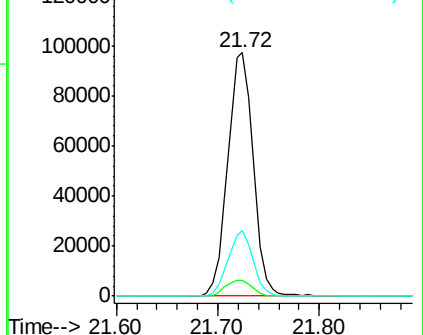

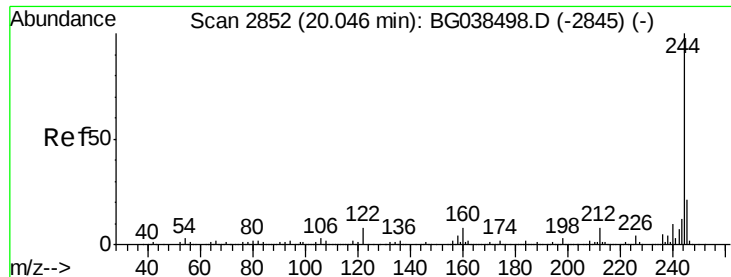

#79

Terphenyl-d14

Concen: 99.563 ng

RT: 20.04 min Scan# 2886

Delta R.T. -0.00 min

Lab File: BG038659.D

Acq: 17 Dec 2018 12:25

Instrument :

BNA_G

ClientSampleId :

P001-SS004-1824-01


Tgt Ion:244 Resp: 775188

Ion Ratio Lower Upper

244 100

212 7.9 6.2 9.2




122 7.5 6.3 9.5

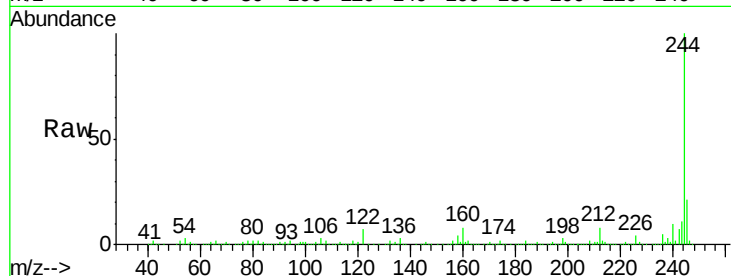

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

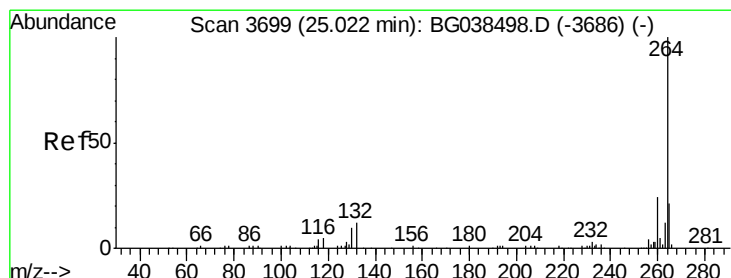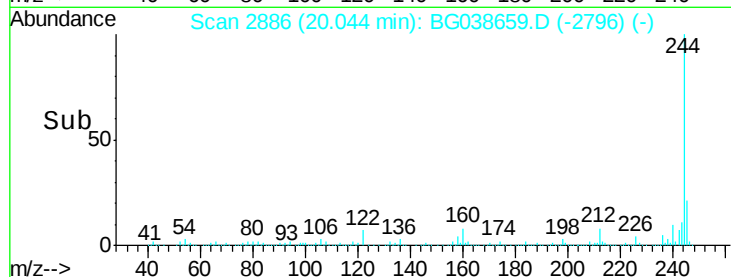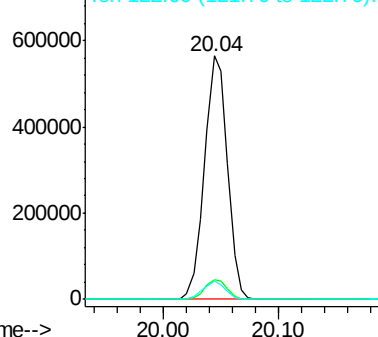

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.02 min Scan# 3733

Delta R.T. -0.00 min

Lab File: BG038659.D

Acq: 17 Dec 2018 12:25


Tgt Ion:264 Resp: 176580

Ion Ratio Lower Upper

264 100

260 22.2 18.9 28.3

265 20.1 17.0 25.4

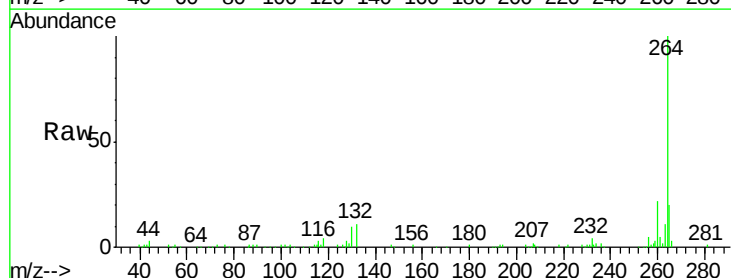

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

