

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG121718\
 Data File : BG038674.D
 Acq On : 17 Dec 2018 23:00
 Operator : JU/SJ
 Sample : J6346-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DW-11

Quant Time: Dec 18 03:43:03 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 12 15:26:27 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	19916	20.00	ng	0.00
21) Naphthalene-d8	10.88	136	80670	20.00	ng	0.00
39) Acenaphthene-d10	14.69	164	56150	20.00	ng	0.00
64) Phenanthrene-d10	17.44	188	146260	20.00	ng	0.00
76) Chrysene-d12	21.72	240	140573	20.00	ng	0.00
87) Perylene-d12	25.02	264	158520	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	168787	150.32	ng	0.00
7) Phenol-d6	7.21	99	231970	150.48	ng	0.00
23) Nitrobenzene-d5	9.23	82	152437	96.54	ng	0.00
42) 2,4,6-Tribromophenol	16.19	330	116391	150.41	ng	0.00
45) 2-Fluorobiphenyl	13.32	172	356914	87.20	ng	0.00
79) Terphenyl-d14	20.04	244	638662	98.88	ng	0.00
Target Compounds						
10) Phenol	7.24	94	15160	9.257	ng	98
50) Dimethylphthalate	14.14	163	30268	6.601	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG121718\
Data File : BG038674.D
Acq On : 17 Dec 2018 23:00
Operator : JU/SJ
Sample : J6346-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DW-11

Quant Time: Dec 18 03:43:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

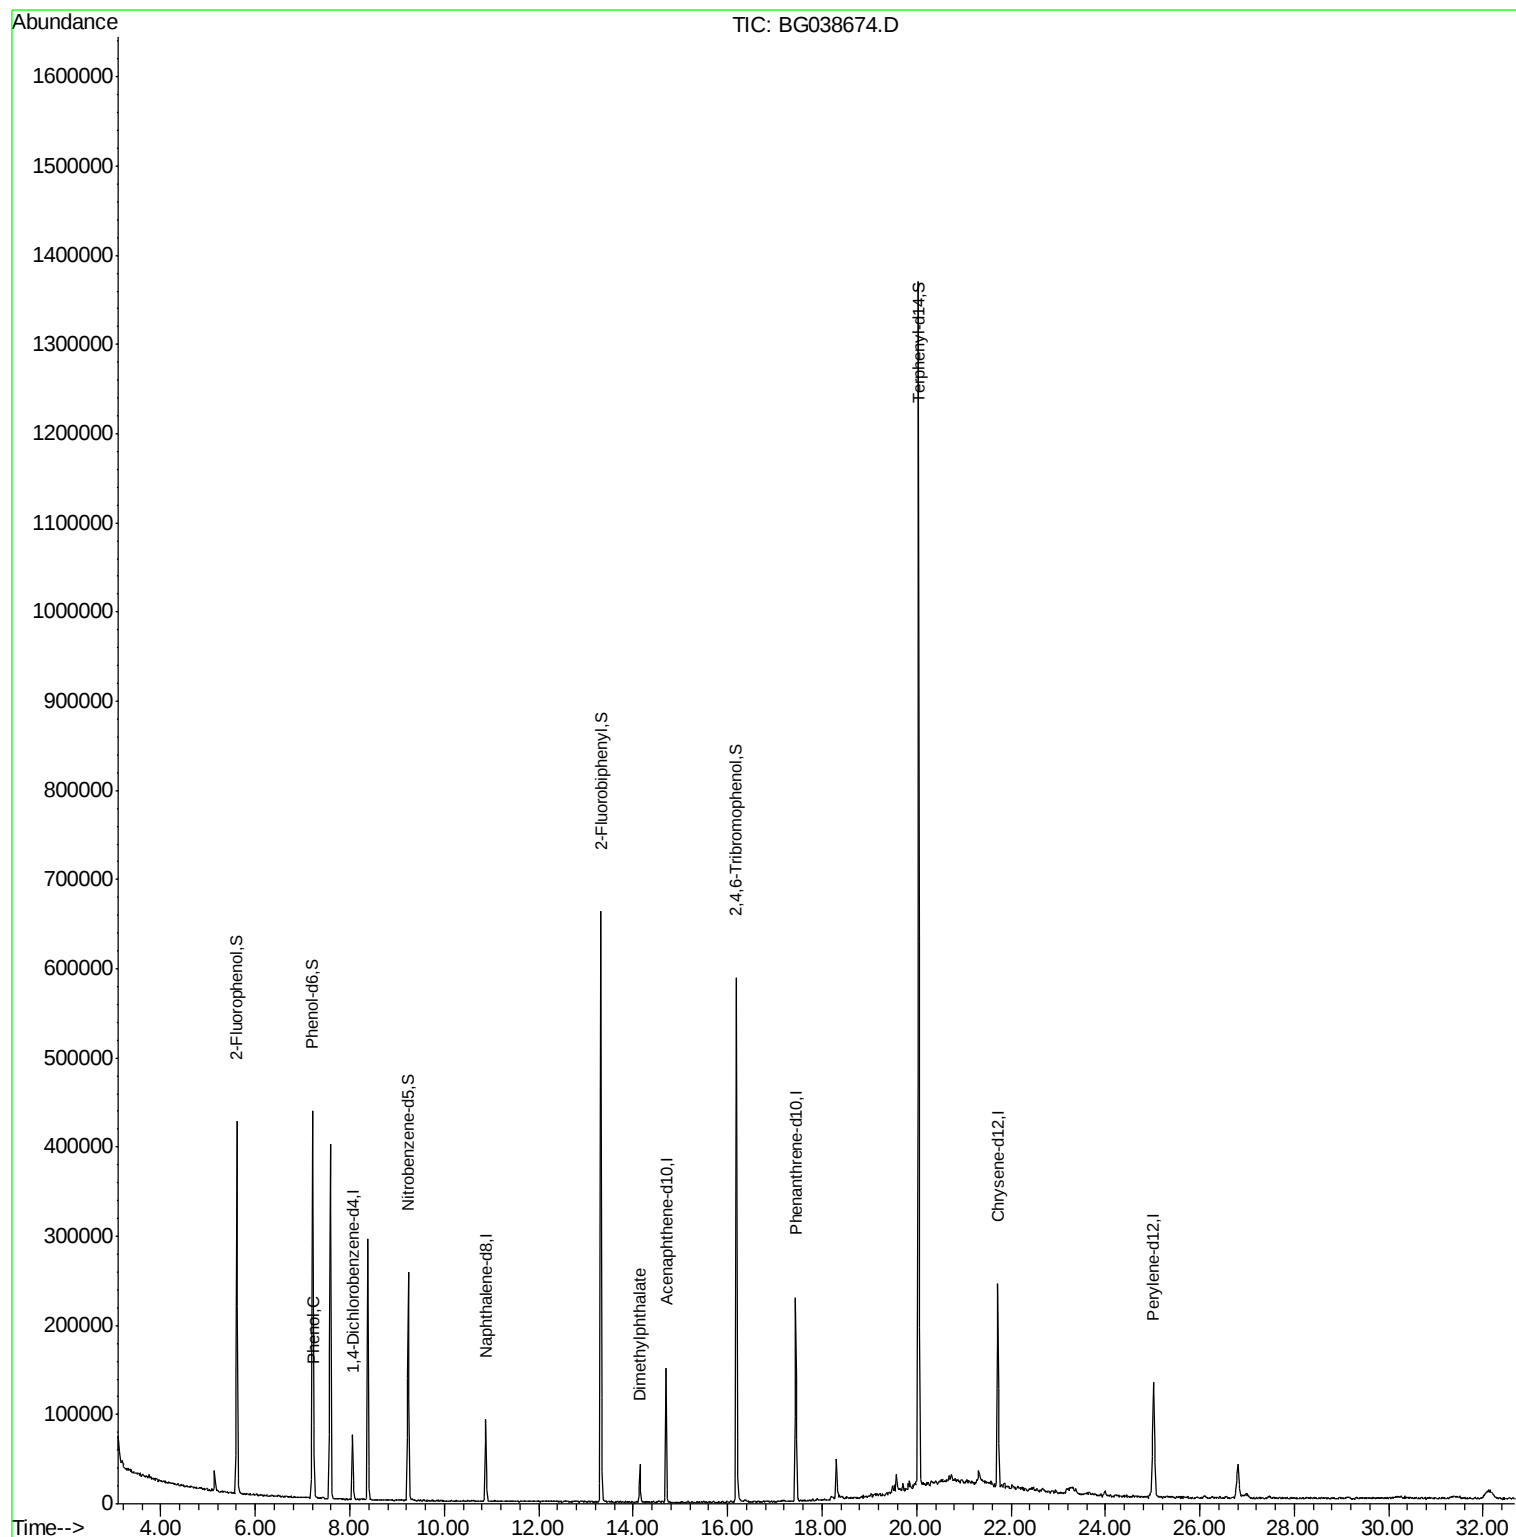



#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.06 min Scan# 846

Delta R.T. -0.00 min

Lab File: BG038674.D

Acq: 17 Dec 2018 23:00

Instrument :

BNA_G

ClientSampleId :

DW-11


Tgt Ion:152 Resp: 19916

Ion Ratio Lower Upper

152 100

150 159.3 119.5 179.3




115 62.7 49.6 74.4

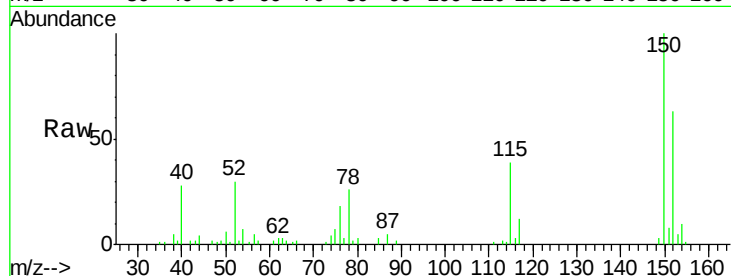

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

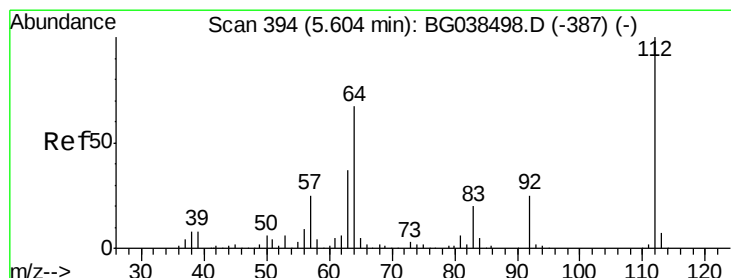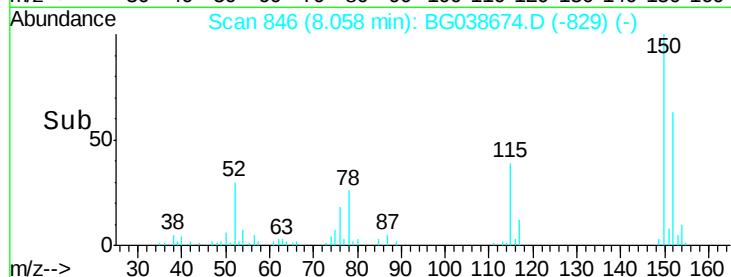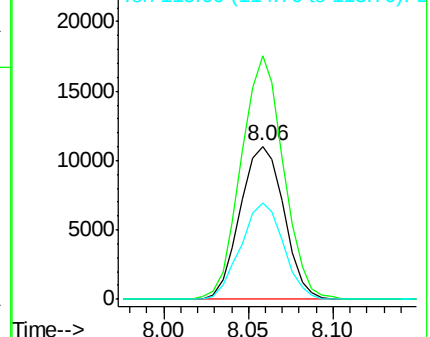

#5

2-Fluorophenol

Concen: 150.316 ng

RT: 5.61 min Scan# 429

Delta R.T. 0.01 min

Lab File: BG038674.D

Acq: 17 Dec 2018 23:00


Tgt Ion:112 Resp: 168787

Ion Ratio Lower Upper

112 100

64 70.0 53.4 80.2



63 41.5 29.3 43.9

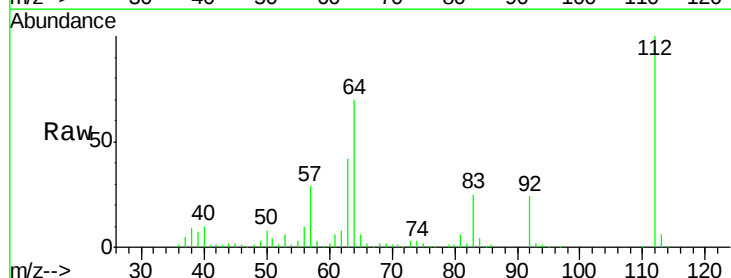


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

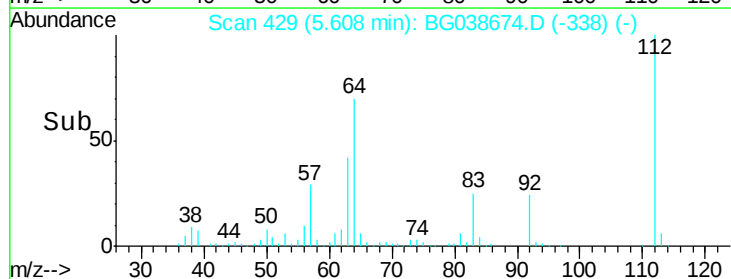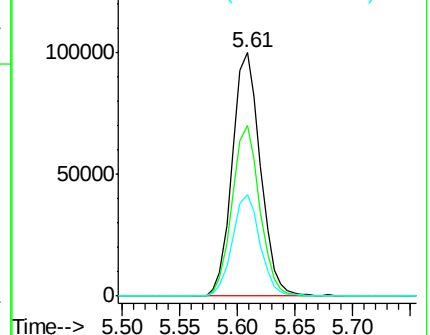

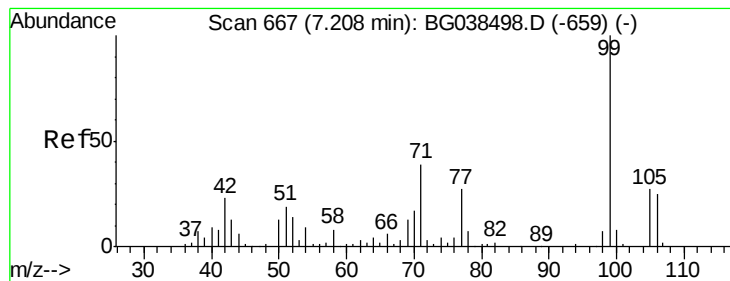

#7

Phenol-d6

Concen: 150.483 ng

RT: 7.21 min Scan# 702

Delta R.T. 0.00 min

Lab File: BG038674.D

Acq: 17 Dec 2018 23:00

Instrument :

BNA_G

ClientSampleId :

DW-11


Tgt Ion: 99 Resp: 231970

Ion Ratio Lower Upper




99 100

42 25.3 18.5 27.7

71 41.1 31.1 46.7

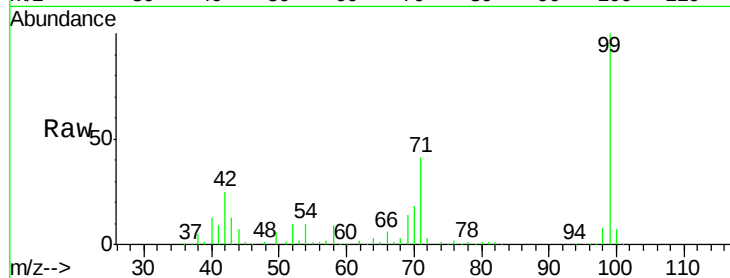

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

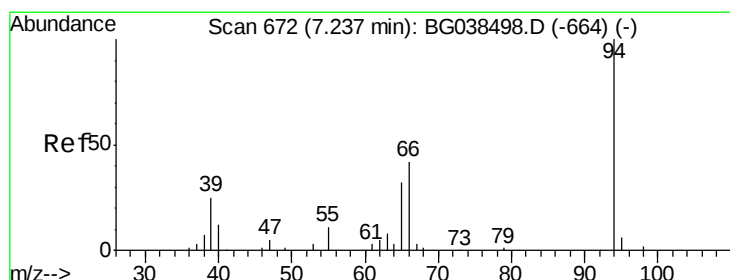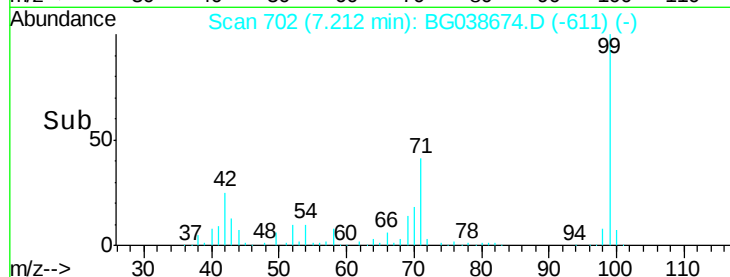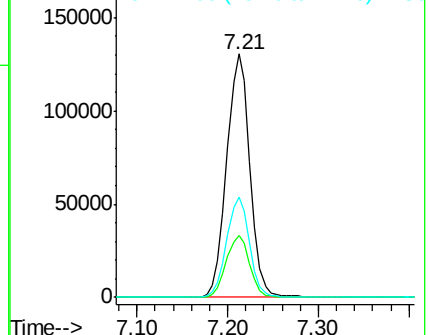

#10

Phenol

Concen: 9.257 ng

RT: 7.24 min Scan# 707

Delta R.T. 0.00 min

Lab File: BG038674.D

Acq: 17 Dec 2018 23:00


Tgt Ion: 94 Resp: 15160

Ion Ratio Lower Upper



94 100

65 30.3 12.6 52.6

66 44.4 24.1 64.1

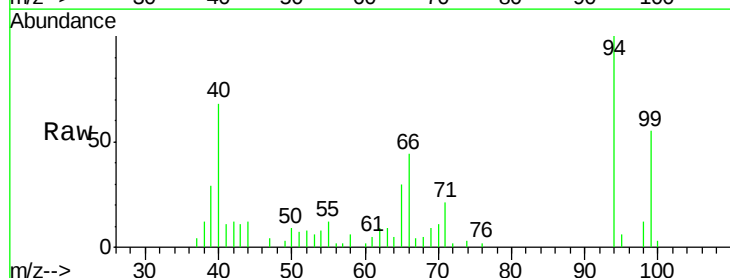

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

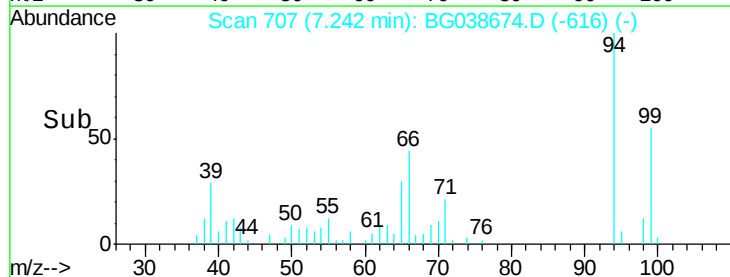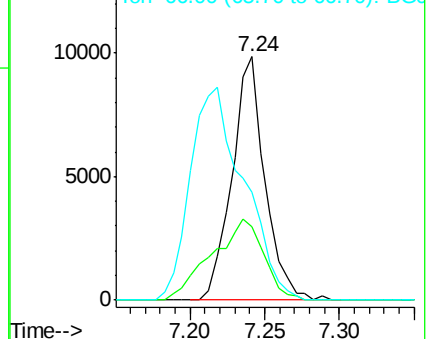







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.88 min Scan# 1326
Delta R.T. -0.00 min
Lab File: BG038674.D
Acq: 17 Dec 2018 23:00

Instrument :
BNA_G
ClientSampleId :
DW-11

Tgt Ion:	136	Resp:	80670
Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.3	13.9
54	10.5	8.5	12.7
68	4.7	3.5	5.3

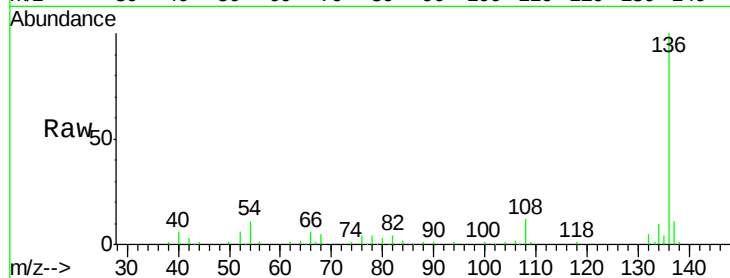


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

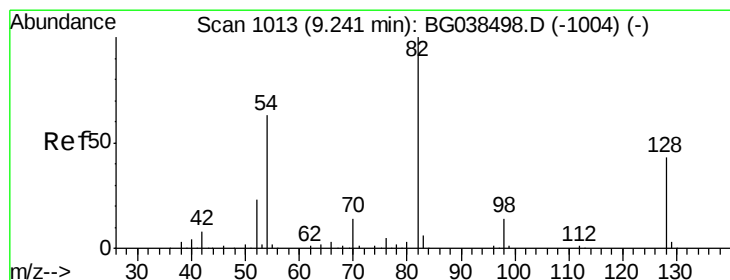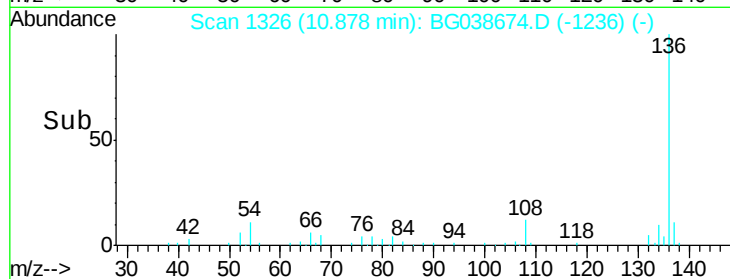
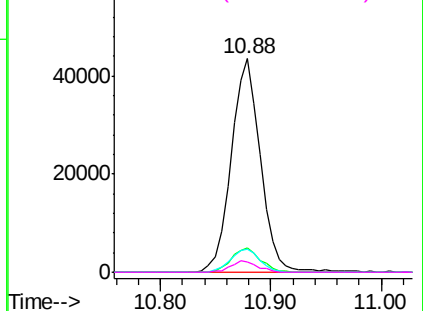



#23
Nitrobenzene-d5
Concen: 96.536 ng
RT: 9.23 min Scan# 1046
Delta R.T. -0.01 min
Lab File: BG038674.D
Acq: 17 Dec 2018 23:00

Tgt Ion:	82	Resp:	152437
Ion	Ratio	Lower	Upper
82	100		
128	40.3	34.6	52.0
54	62.8	50.6	76.0

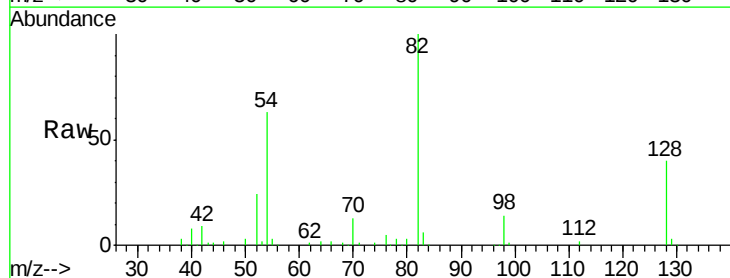

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

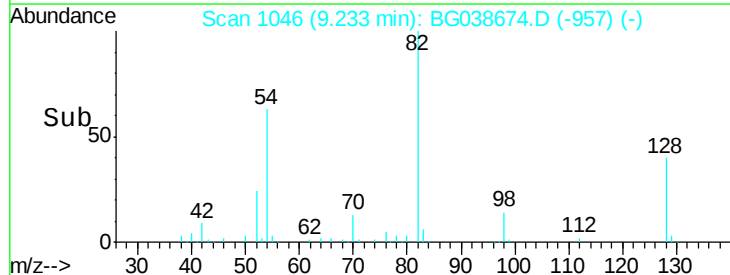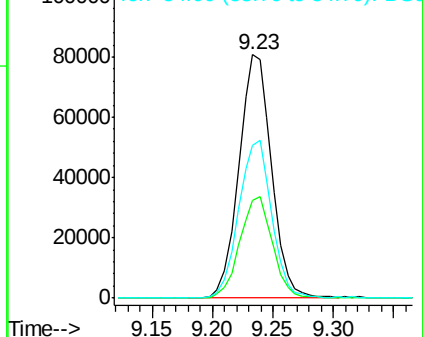

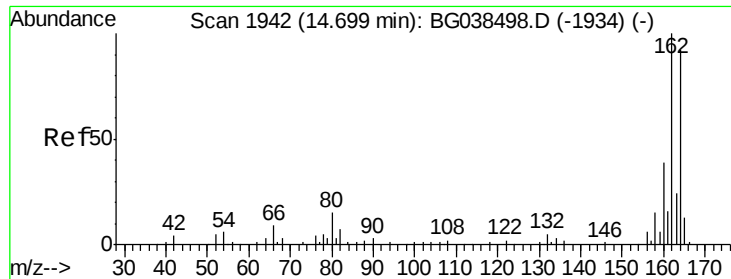

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.69 min Scan# 1975

Delta R.T. -0.01 min

Lab File: BG038674.D

Acq: 17 Dec 2018 23:00

Instrument :

BNA_G

ClientSampled :

DW-11


Tgt Ion:164 Resp: 56150

Ion Ratio Lower Upper

164 100

162 101.6 86.6 130.0




160 43.8 34.2 51.2

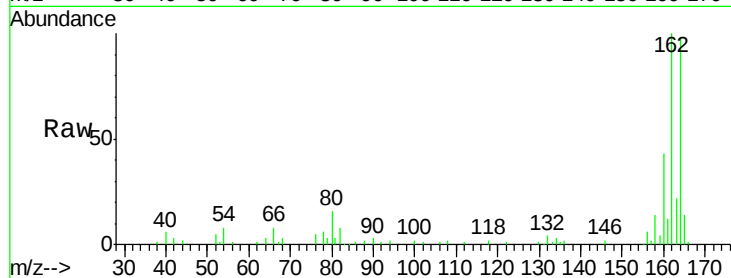

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

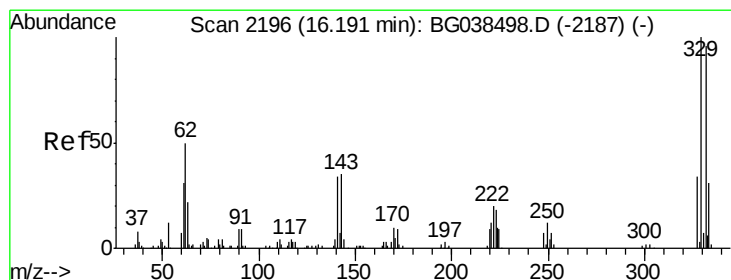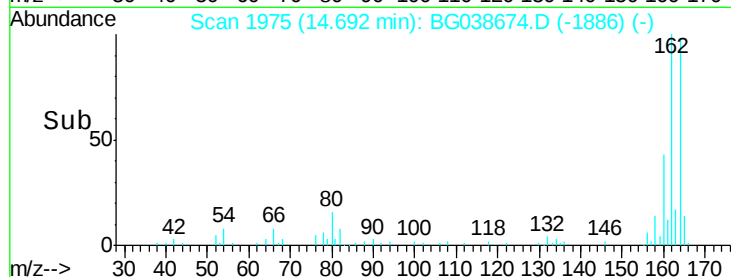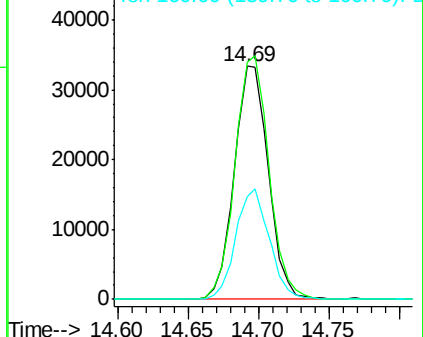

#42

2,4,6-Tribromophenol

Concen: 150.405 ng

RT: 16.19 min Scan# 2230

Delta R.T. -0.00 min

Lab File: BG038674.D

Acq: 17 Dec 2018 23:00


Tgt Ion:330 Resp: 116391

Ion Ratio Lower Upper

330 100

332 96.0 76.9 115.3



141 38.0 28.8 43.2

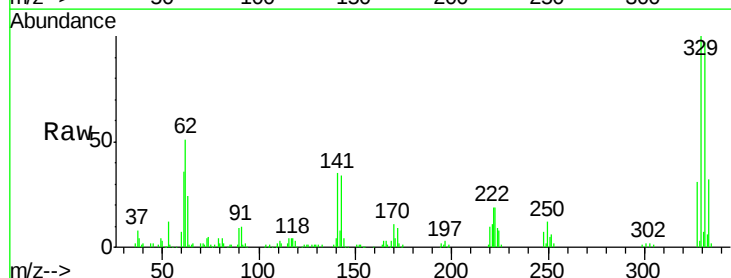


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



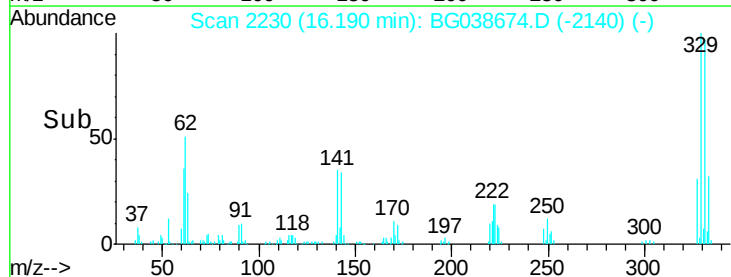
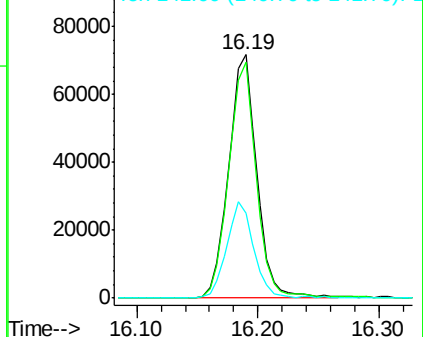


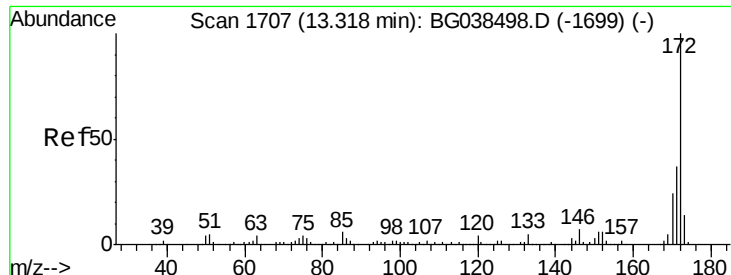

#45
2-Fluorobiphenyl
Concen: 87.201 ng
RT: 13.32 min Scan# 1741
Delta R.T. -0.00 min
Lab File: BG038674.D
Acq: 17 Dec 2018 23:00




Instrument :
BNA_G
ClientSampleId :
DW-11


Tgt Ion:172 Resp: 356914
Ion Ratio Lower Upper
172 100
171 37.5 29.8 44.6
170 26.1 19.5 29.3

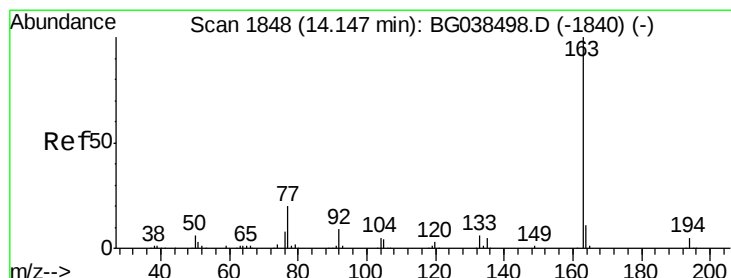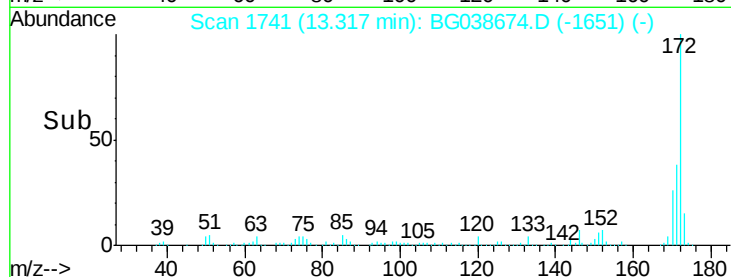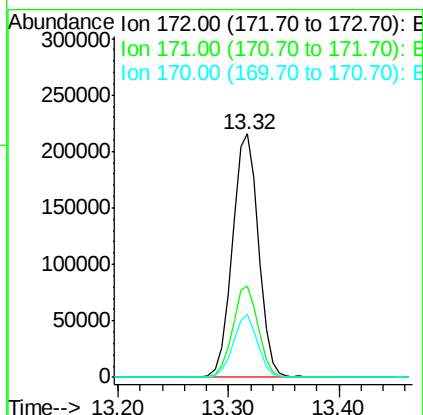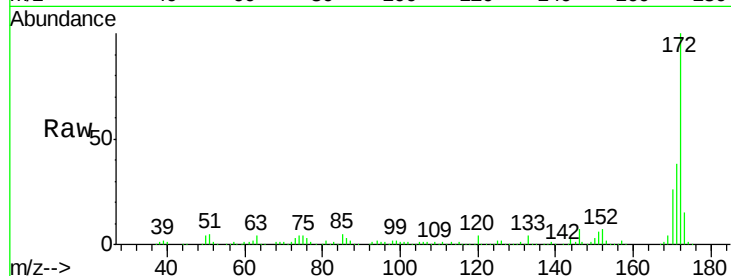

#50
Dimethylphthalate
Concen: 6.601 ng
RT: 14.14 min Scan# 1881
Delta R.T. -0.01 min
Lab File: BG038674.D
Acq: 17 Dec 2018 23:00

Tgt Ion:163 Resp: 30268
Ion Ratio Lower Upper
163 100
194 4.6 3.7 5.5
164 10.2 8.6 12.8

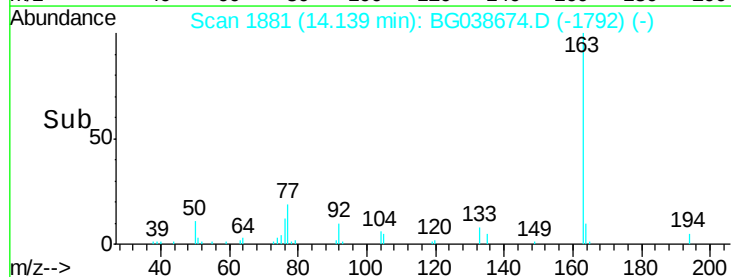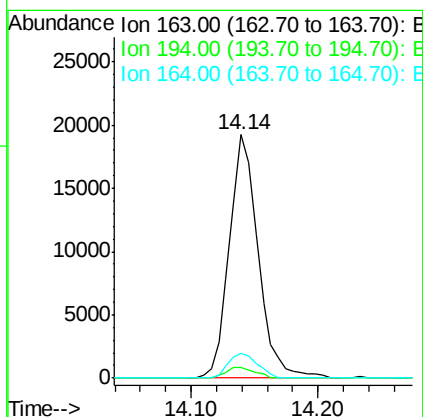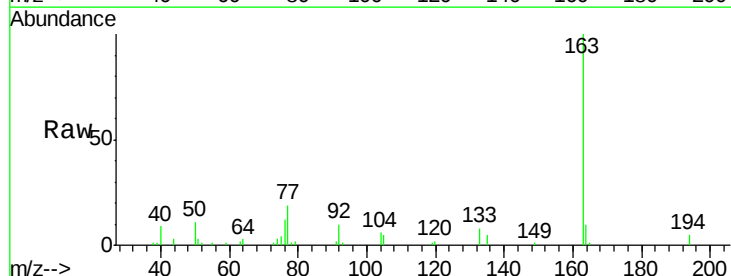

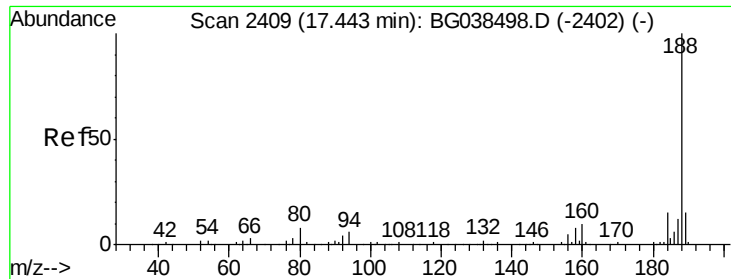

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.44 min Scan# 2443

Delta R.T. -0.00 min

Lab File: BG038674.D

Acq: 17 Dec 2018 23:00

Instrument :

BNA_G

ClientSampleId :

DW-11


Tgt Ion:188 Resp: 146260

Ion Ratio Lower Upper

188 100

94 6.4 5.1 7.7




80 6.6 6.1 9.1

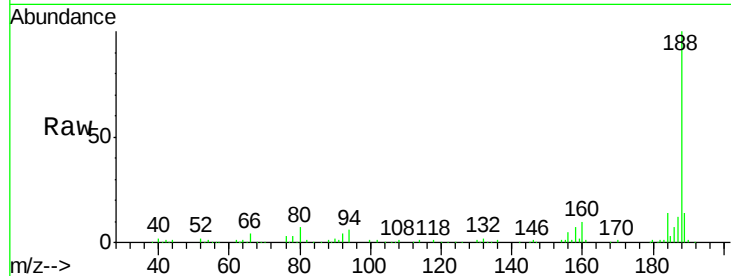

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

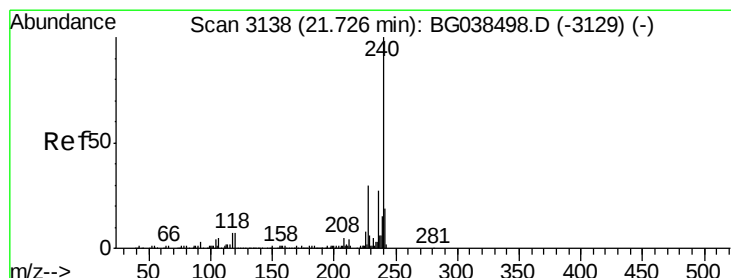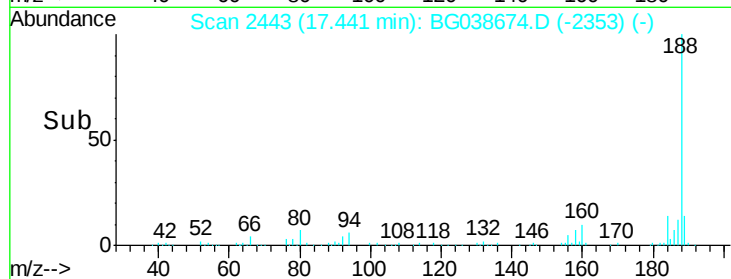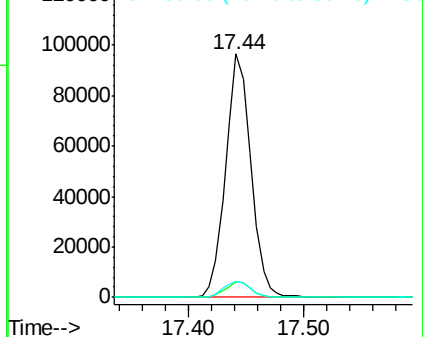

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.72 min Scan# 3172

Delta R.T. -0.00 min

Lab File: BG038674.D

Acq: 17 Dec 2018 23:00


Tgt Ion:240 Resp: 140573

Ion Ratio Lower Upper

240 100

120 6.0 5.3 7.9



236 26.4 21.4 32.2

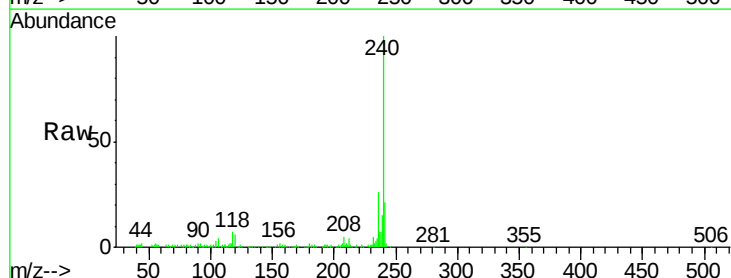


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

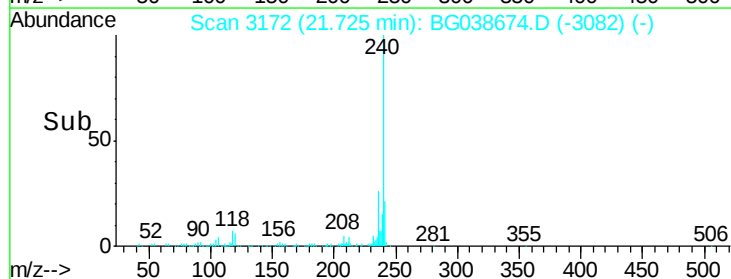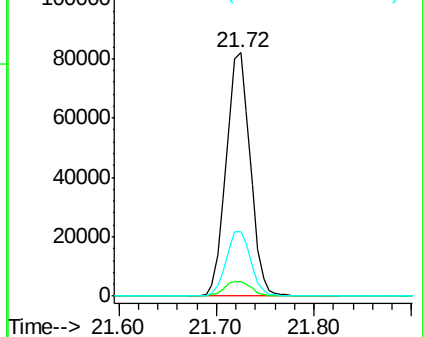

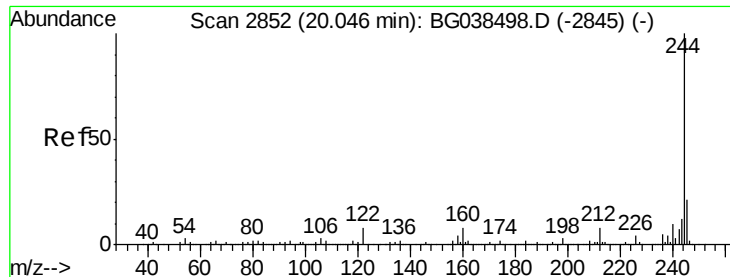

#79

Terphenyl-d14

Concen: 98.877 ng

RT: 20.04 min Scan# 2886

Delta R.T. -0.00 min

Lab File: BG038674.D

Acq: 17 Dec 2018 23:00

Instrument :

BNA_G

ClientSampleId :

DW-11


Tgt Ion:244 Resp: 638662

Ion Ratio Lower Upper

244 100

212 7.9 6.2 9.2




122 6.9 6.3 9.5

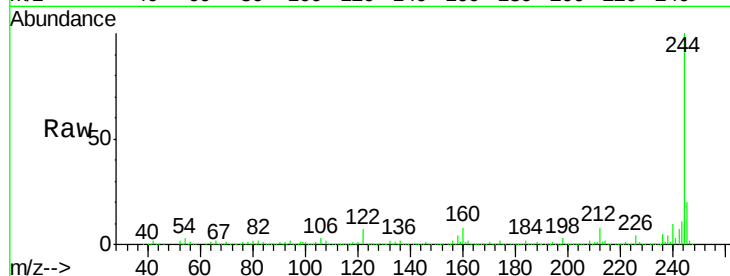

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

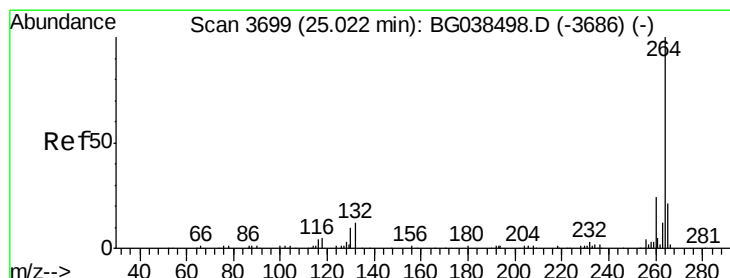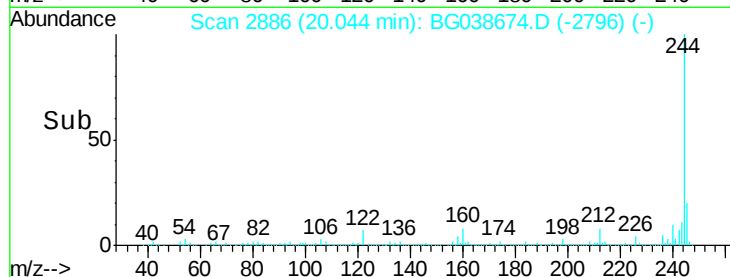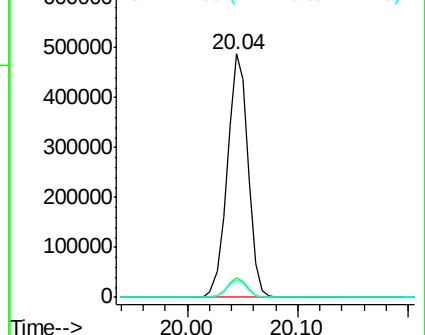

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.02 min Scan# 3733

Delta R.T. -0.00 min

Lab File: BG038674.D

Acq: 17 Dec 2018 23:00


Tgt Ion:264 Resp: 158520

Ion Ratio Lower Upper

264 100

260 21.5 18.9 28.3

265 19.7 17.0 25.4

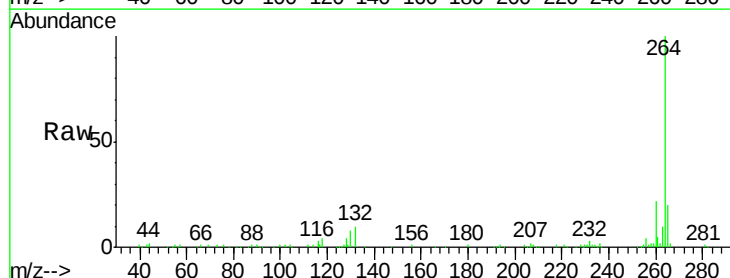

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

