


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG121718\
 Data File : BG038672.D
 Acq On : 17 Dec 2018 21:40
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

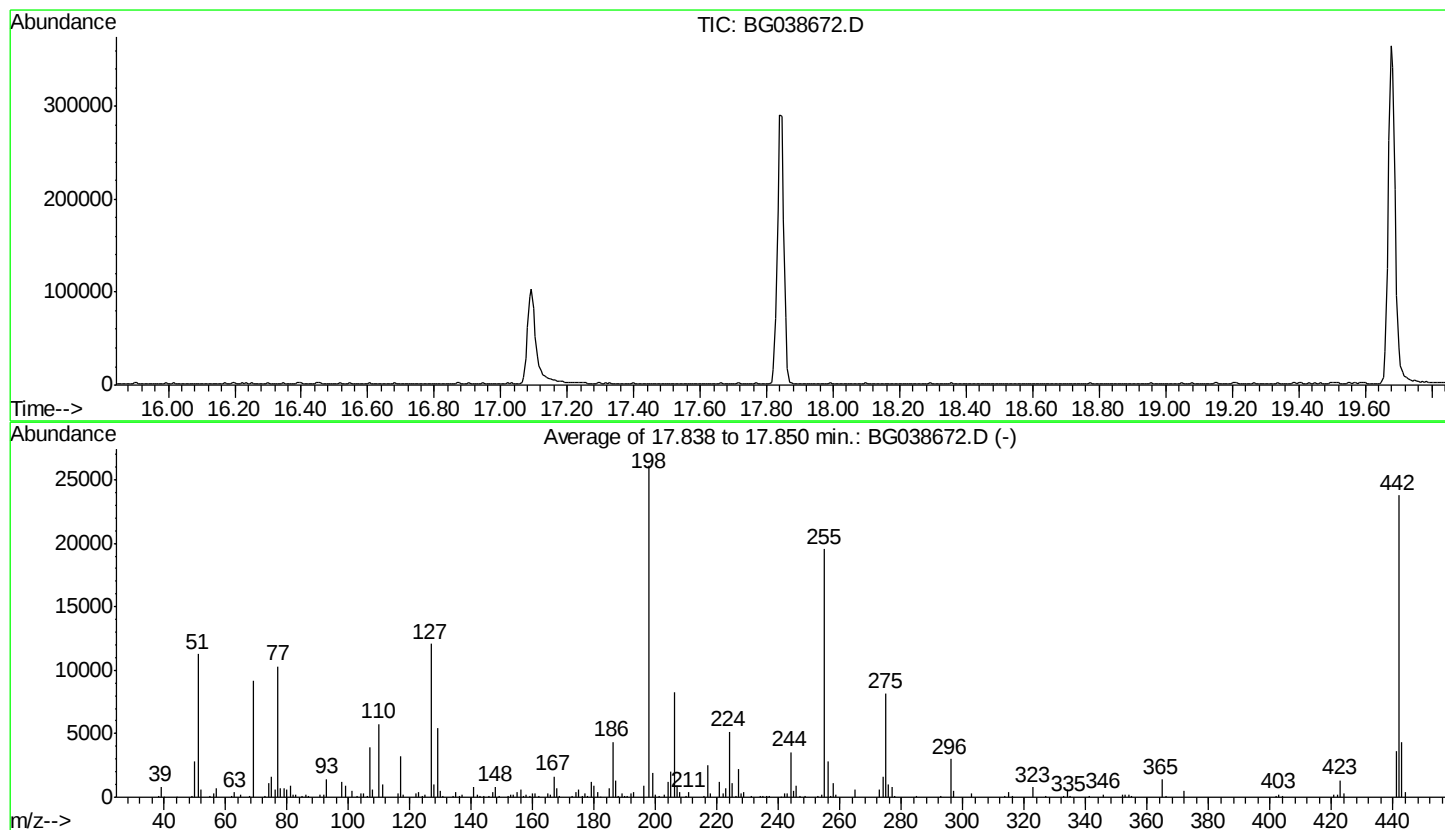

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	11248	PASS
68	69	0.00	2	1.3	115	PASS
69	198	0.00	100	35.0	9151	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.2	12074	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26109	PASS
199	198	5	9	7.4	1923	PASS
275	198	10	60	31.2	8134	PASS
365	198	1	100	5.3	1385	PASS
441	198	0.01	100	13.8	3613	PASS
442	198	50	100	91.0	23754	PASS
443	442	15	24	18.4	4379	PASS