


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121719\
 Data File : BG043814.D
 Acq On : 17 Dec 2019 11:04
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 09 18:16:57 2019

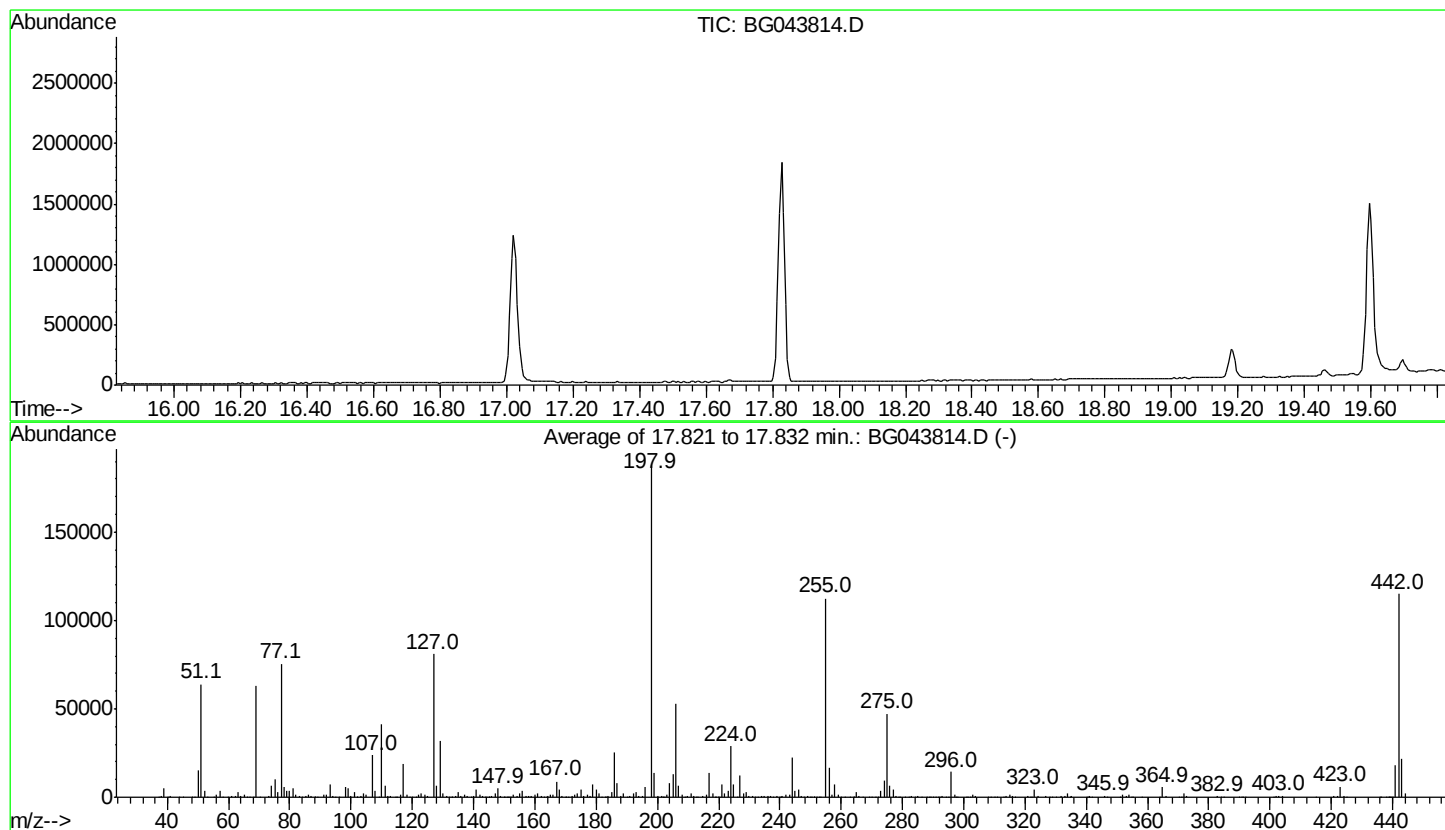

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	64077	PASS
68	69	0.00	2	0.3	212	PASS
69	198	0.00	100	33.5	62778	PASS
70	69	0.00	2	0.2	115	PASS
127	198	10	80	43.2	81056	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	187541	PASS
199	198	5	9	7.3	13771	PASS
275	198	10	60	25.1	47144	PASS
365	198	1	100	3.0	5577	PASS
441	198	0.01	100	9.7	18110	PASS
442	198	50	100	61.2	114826	PASS
443	442	15	24	18.7	21493	PASS