


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121720\
 Data File : BG047759.D
 Acq On : 17 Dec 2020 9:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 17 15:55:16 2020

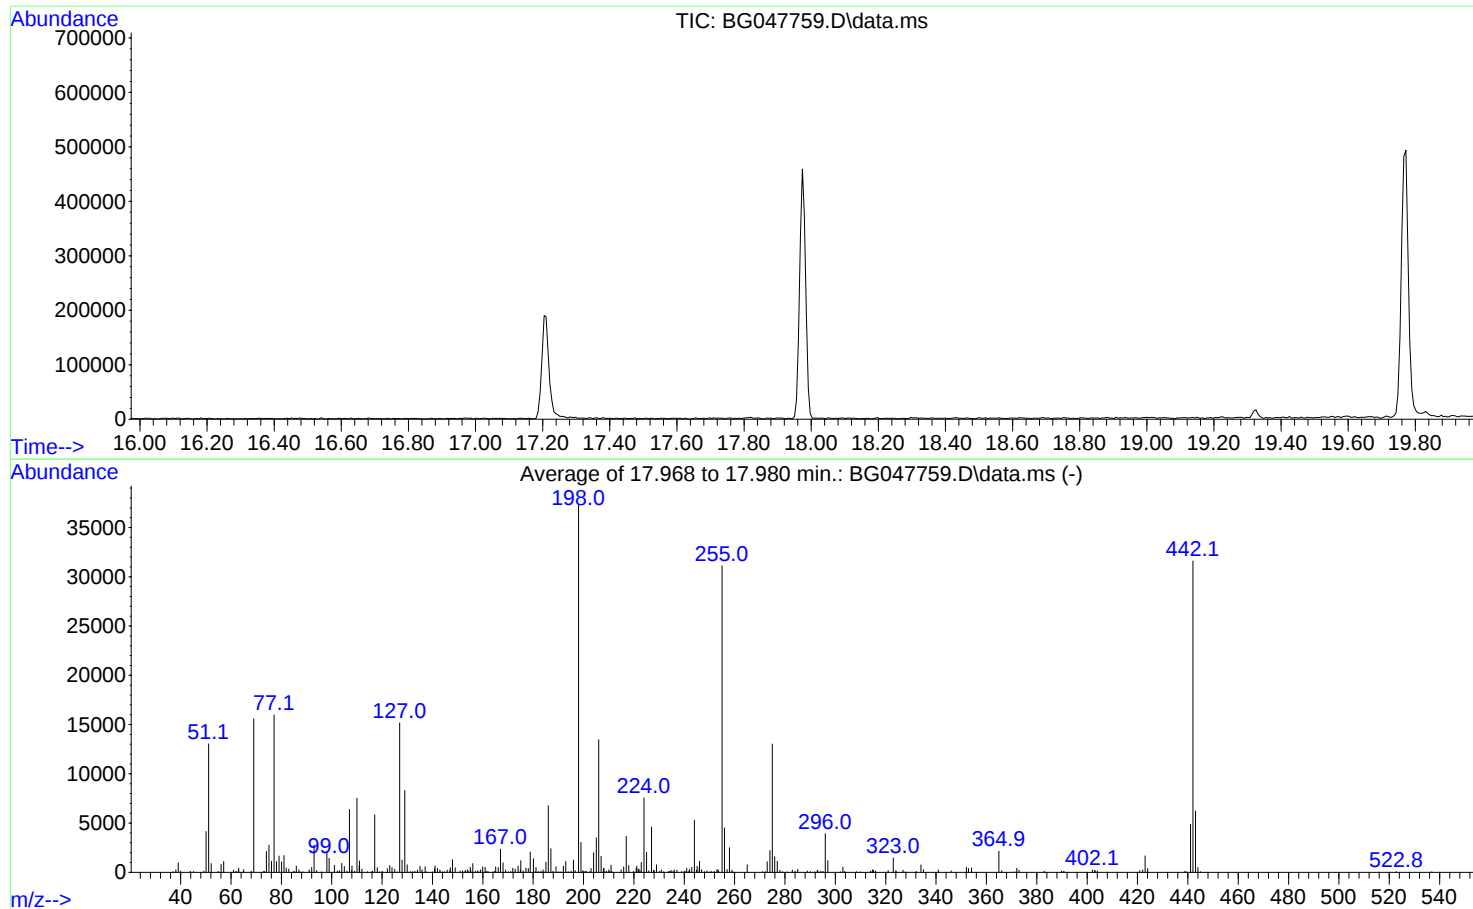

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	13048	PASS
68	69	0.00	2	0.8	123	PASS
69	198	0.00	100	41.8	15588	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.6	15166	PASS
197	198	0.00	2	0.5	182	PASS
198	198	100	100	100.0	37333	PASS
199	198	5	9	8.1	3032	PASS
275	198	10	60	34.9	13029	PASS
365	198	1	100	5.8	2153	PASS
441	198	0.01	100	13.0	4868	PASS
442	198	50	100	84.6	31595	PASS
443	442	15	24	19.7	6217	PASS