
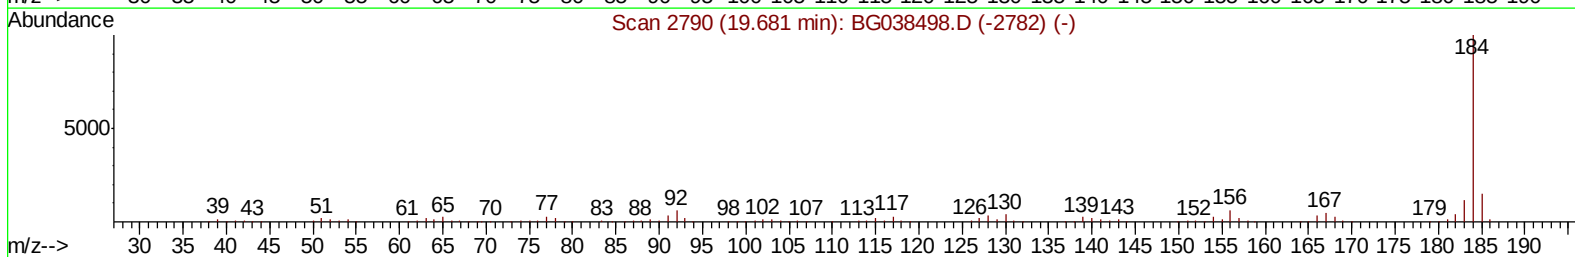
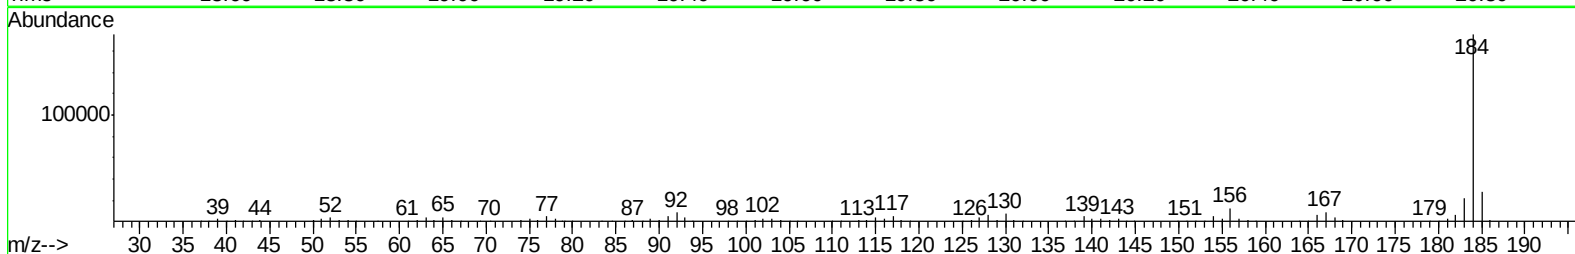


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG121818\
 Data File : BG038691.D
 Acq On : 18 Dec 2018 11:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 08:06:36 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 12 15:26:27 2018
 Response via : Initial Calibration

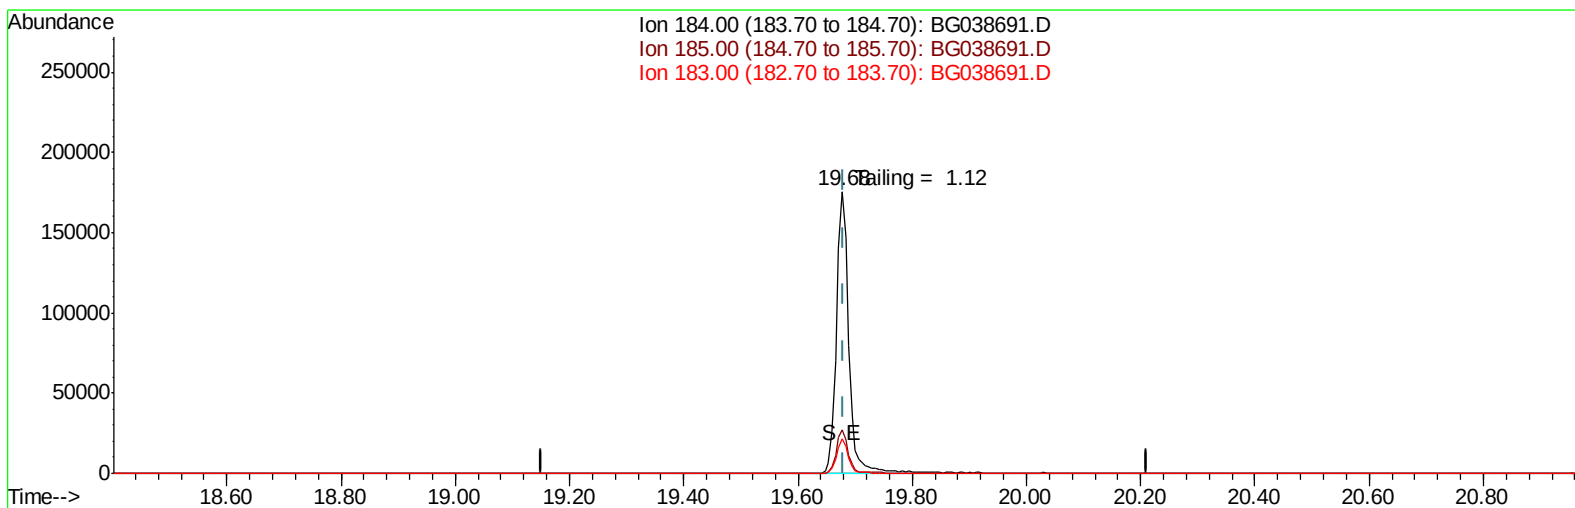

TIC: BG038691.D

(77) Benzidine




19.677min (-0.004) 0.00ng

response 262482

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.60
183.00	12.00	12.46
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG121818\
Data File : BG038691.D
Acq On : 18 Dec 2018 11:25
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 08:06:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

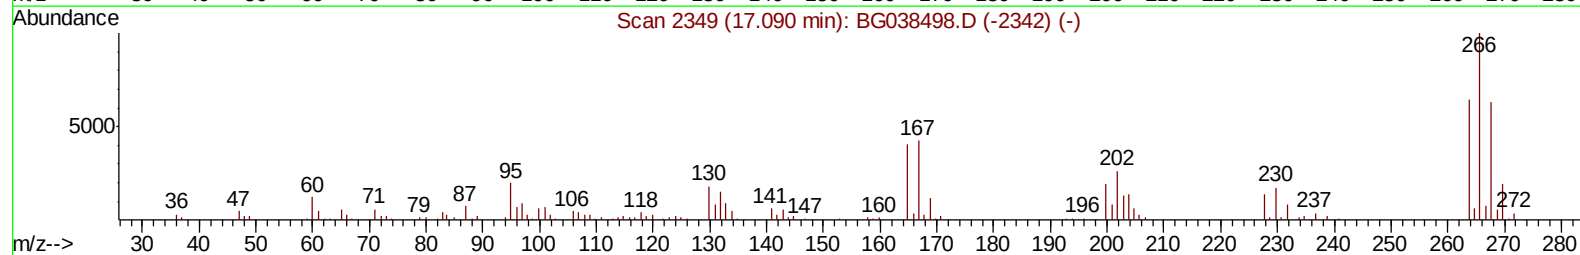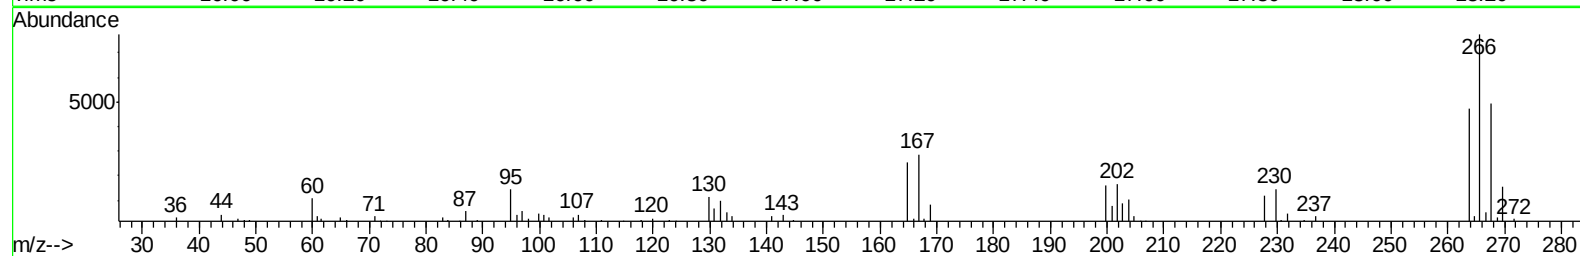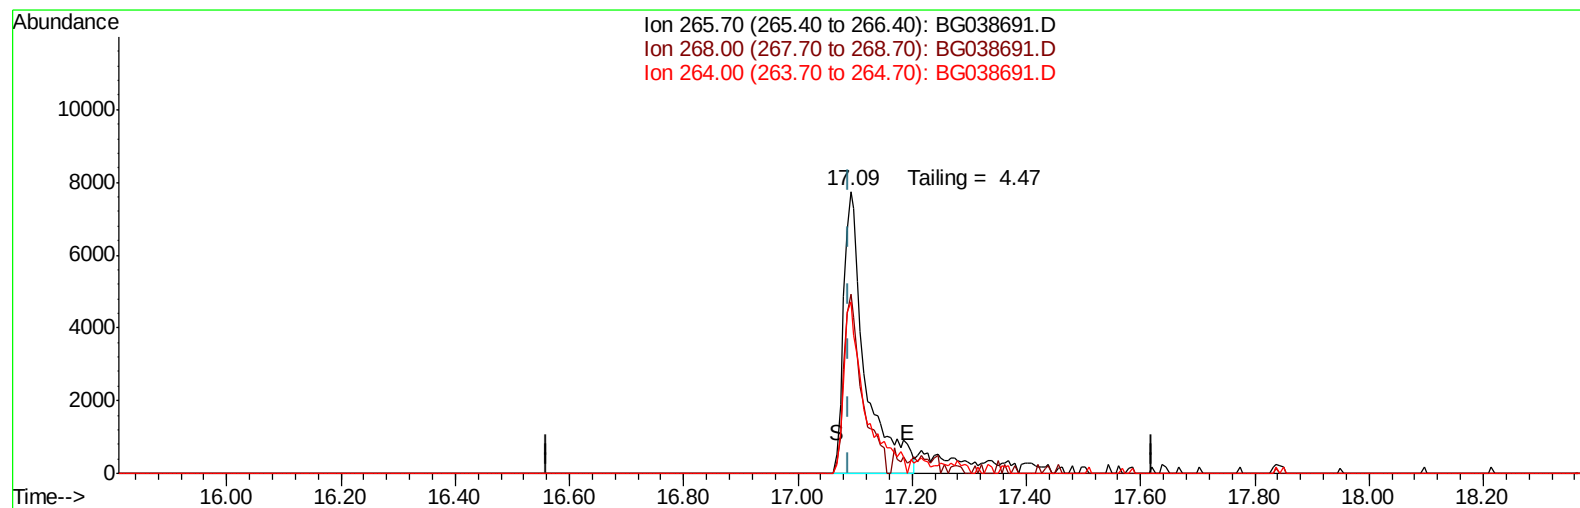

TIC: BG038691.D

(70) Pentachlorophenol (C)

17.092min (+0.002) 18428.91ng

response 20286

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	63.74
264.00	70.90	65.25
0.00	0.00	0.00